

Southern Ocean diatoms and climate change: quantifying the relative roles of diversity and plasticity in evolution. (Rynearson)

Southern Ocean Carbon and climate Observations and Modeling. (Sarmiento)

Pathways of Circumpolar Deep Water to West Antarctica from profiling float and satellite measurements. (Girton)

# Data Report NBP1701

RVIB Nathaniel B. Palmer

December 24<sup>th</sup>, 2016 – January 20<sup>th</sup>, 2017



*Photo by Pablo Cohn*

United States Antarctic Program

Data Report Prepared By:  
Scott Walker  
David "Pablo" Cohn

## Table of Contents

<b>Introduction.....</b>	<b>1</b>
Distribution Contents at a Glance.....	2
Extracting Data.....	3
<b>Distribution Contents.....</b>	<b>4</b>
Cruise Track.....	4
Satellite Images.....	4
NBP Data Products.....	4
JGOFS.....	5
MGD77.....	6
<b>Science of Opportunity.....</b>	<b>8</b>
ADCP.....	8
pCO <sub>2</sub> .....	8
<b>Cruise Science.....</b>	<b>9</b>
CTD.....	9
XBT.....	9
RVDAS.....	9
Sensors and Instruments.....	9
Underway Sensors.....	10
<i>Meteorology and Radiometry.....</i>	<i>10</i>
<i>Geophysics.....</i>	<i>10</i>
<i>Oceanography.....</i>	<i>10</i>
<i>Navigational Instruments.....</i>	<i>10</i>
<b>Data.....</b>	<b>11</b>
Underway Data.....	12
<i>Sound Velocity Probe (svp1).....</i>	<i>12</i>
<i>Meteorology (mwx1).....</i>	<i>12</i>
<i>Knudsen (knud).....</i>	<i>13</i>
<i>Gravimeter (grv1).....</i>	<i>13</i>
<i>pCO<sub>2</sub> (pco2).....</i>	<i>14</i>
<i>Micro TSG (tsg1, tsg2).....</i>	<i>14</i>
<i>Remote Temperature (rtmp).....</i>	<i>14</i>
<i>GUV (pguv).....</i>	<i>15</i>
<i>Engineering (eng1).....</i>	<i>15</i>
<i>Hydro DAS (hdas).....</i>	<i>16</i>
<i>Winch (bwnc, cwnc, twnc).....</i>	<i>16</i>
<i>Multibeam (mbdp).....</i>	<i>16</i>
Navigational Data.....	17
<i>GPS (s330, seap, PCOD).....</i>	<i>17</i>
<i>Gyro Compass (gyr1).....</i>	<i>22</i>
Processed Data.....	23

<i>pCO<sub>2</sub> – Merged</i> .....	23
Calculations .....	24
<i>PAR</i> .....	24
<i>PSP</i> .....	24
<i>PIR</i> .....	25
<b>Acquisition Problems and Events</b> .....	<b>26</b>
<b>Appendix A: Sensors</b> .....	<b>27</b>
NBP1701 Sensors .....	27
<i>Meteorology and Radiometry</i> .....	27
<i>Underway Seawater Sampling System</i> .....	27
<i>CTD</i> .....	27
<b>Appendix B: Calibration Sheets</b> .....	<b>28</b>
Gravity .....	28
Meteorology .....	29
<i>Anemometers</i> .....	29
<i>Barometer</i> .....	30
<i>Temperature / Humidity</i> .....	31
<i>PIR</i> .....	32
<i>PSP</i> .....	33
<i>PAR (Mast)</i> .....	34
<i>GUV (Mast)</i> .....	35
Underway Seawater Sampling System .....	36
<i>Micro-TSG 2</i> .....	36
<i>Micro-TSG1</i> .....	38
<i>Digital Remote Temp</i> .....	41
<i>Transmissometer</i> .....	43
<i>Fluorometer</i> .....	44
CTD .....	45
<i>Altimeter</i> .....	45
<i>Conductivity (primary)</i> .....	46
<i>Conductivity (secondary)</i> .....	47
<i>Fluorometer</i> .....	48
<i>PAR</i> .....	49
<i>Pressure Sensor</i> .....	50
<i>Dissolved Oxygen (primary)</i> .....	52
<i>Pump (primary)</i> .....	53
<i>Pump (secondary)</i> .....	54
<i>Temperature (primary)</i> .....	55
<i>Temperature (Secondary)</i> .....	56
<i>Transmissometer</i> .....	57

## Introduction

The NBP data acquisition systems continuously log data from the instruments used during the cruise. This document describes:

- The structure and organization of the data on the distribution media
- The format and contents of the data strings
- Formulas for calculating values
- Information about the specific instruments in use during the cruise
- A log of acquisition problems and events during the cruise that may affect the data
- Scanned calibration sheets for the instruments in use during the cruise.

The data is distributed on a DVD+R or CD-ROM written in ISO9660 level-1 format. It is readable by virtually every computing platform.

All the data has been archived using 'tar' and compressed using 'gzip', identified by the '.tz' extension. Tools are available on all platforms for uncompressing and de-archiving these formats: On Macintosh use the built-in Archive Utility, or tar in the terminal. On Windows operating systems use WinZip or 7Zip.

MultiBeam and Bathymetry data, if collected, are distributed separately.

*IMPORTANT: Read the last section, "Acquisition Problems and Events," for important information that may affect the processing of this data.*

## Distribution Contents at a Glance

### Volume 1 of 1: NBP1701

#### File

```

/
  NBP1701.gmt
  NBP1701.mgd
  NBP1701.trk
  NBP1701DATA.docx
  NBP1701DATA.pdf
  INSTCOEF.TXT
/process
  NBP1701JGOF.tz
  NBP1701MGD.tz
  NBP1701PCO2.tz
  NBP1701PROC.tz
  NBP1701QC.tz
/rvdas/nav
  NBP1701adcp.tz
  NBP1701PCOD.tz
  NBP1701gyr1.tz
  NBP1701s330.tz
  NBP1701seap.tz
/rvdas/uw
  NBP1701bwnc.tz
  NBP1701ctdd.tz
  NBP1701engl.tz
  NBP1701grv1.tz
  NBP1701hdas.tz
  NBP1701knud.tz
  NBP1701mbdp.tz
  NBP1701mwx1.tz
  NBP1701pco2.tz
  NBP1701pguv.tz
  NBP1701rtmp.tz
  NBP1701svp1.tz
  NBP1701tsg1.tz
  NBP1701tsg2.tz
  NBP1701twnc.tz
/science
  NBP1701elog.tz
/Imagery
  NBP1701Imag.tz
/ocean
  NBP1701ctd.tz

```

#### Description

```

Root level directory
  GMT binary file of MGD77 data
  Full Cruise MGD77 data file
  Text file of cruise track
  Data Report NBP1701 (MS Word)
  Data Report NBP1701 (PDF format)
  Instrument Coefficient File
Processed data
  JGOFs format data files
  MGD Data
  Merged pCO2 data files
  Other processed data
  Daily RVDAS QC postscript plots
Navigation data
  ADCP Data Sets
  Furuno GP-330B
  Gyro raw data
  Seapath 330 data
  Seapath 200 data
Underway data
  Baltic winch data
  CTD depth data
  Engineering data
  Gravimeter data
  HydroDAS raw data
  Knudsen raw data
  Multi-beam depth
  Meteorology raw data
  pCO2 raw data
  GUV raw data
  Remote Temperature data
  Sound velocity probe (ADCP)
  Micro TSG1 data
  Micro TSG2 data
  Trawl winch data
Cruise specific data
  Elog data
Cruise Imagery
  Collection of Imagery Files
Ocean data
  CTD Data

```

## Extracting Data

The data files will have a “.tz” extension on the filename. The “.tz” extension is for files whose contents have been archived using the “tar” utility and compressed with the “gzip” utility.

An example of creating a compressed archive file:

```
tar -czvf archive_filename files_to_archive
```

An example of listing the files in an archive:

```
tar -tzvf archive_filename
```

An example redirecting the list output to a file, where `contents.list` is the name of the file to create:

```
tar -tzvf archive_filename > contents.list
```

An example extracting all files from the archive:

```
tar -xzvf archive_filename
```

An example extracting specific files from the archive:

```
tar -xzvf archive_filename list_of_files_to_extract
```

## Distribution Contents

### Cruise Track

The distribution DVD includes a GMT cruise track file (NBP1701.trk). It contains the longitude and latitude at one-minute intervals extracted from the NBP1701.gmt file.

### Satellite Images

Satellite Images processed for this cruise can be found in the directory, /Imagery in two subdirectories, ice and wx (weather). Files are named using the convention, IdDDDYA.jpg where:

Id = image type (ice = ice, wx = weather)

DDD = year-day

YY = year

A = allows for multiple images of one type for one day

### NBP Data Products

Two datasets are created on each cruise: JGOFS and MGD77.

The data processing scripts used to produce JGOFS and MGD77 data sets create a lot of intermediate files. These files are included on the data distribution media in a file called NBP1701proc.TAR. They are included to make re-processing easier in the event of an error, but no extensive detail of the formats is included in this document. If you have any questions, please contact [itvessel@usap.gov](mailto:itvessel@usap.gov).

## JGOFS

The JGOFS data set can be found on the distribution media in the file /process/NBP1701JGOF.tar. The archive contains one file produced for each day named jgDDD.dat.gz, where DDD is the year-day the data was acquired. The “.gz” extension indicates that the individual files are compressed before archiving. Each daily file consists of 22 columnar fields in text format as described in the table below. The JGOFS data set is created from calibrated data decimated at one-minute intervals. Several fields are derived measurements from more than a single raw input. For example, Course Made Good (CMG) and Speed Over Ground (SOG) are calculated from gyro and GPS inputs. Daily plots during the cruise are produced from the JGOFS data set. Note: Null, unused, or unknown fields are indicated as “NAN” as 9999 in the JGOFS data.

Field	Data	Units
01	UTC Date	dd/mm/yy
02	UTC Time	hh:mm:ss
03	Seapath Latitude (negative is South)	tt.tttt
04	Seapath Longitude (negative is West)	ggg.gggg
05	Speed Over Ground	knots
06	GPS HDOP	-
07	Gyro Heading	Degrees (azimuth)
08	Course Made Good	Degrees (azimuth)
09	Mast PAR	μEinstein's/meter <sup>2</sup>
10	Sea Surface Temperature	°C
11	Sea Surface Conductivity	siemens/meter
12	Sea Surface Salinity	PSU
13	Sea Depth (uncorrected, calc. sw sound vel. 1500 m/s)	meters
14	True Wind Speed (max speed windbird)	meters/sec
15	True Wind Direction (max speed windbird)	degrees (azimuth)
16	Ambient Air Temperature	°C
17	Relative Humidity	%
18	Barometric Pressure	mBars
19	Sea Surface Fluorometry	μg/l
20	Transmissometry	%
21	PSP	W/m <sup>2</sup>
22	PIR	W/m <sup>2</sup>



## MGD77

The MGD77 data set is contained in a single file for the entire cruise. It can be found in the top level of the distribution data structure as NBP1701.mgd. The file NBP1701.gmt is created from the MGD77 dataset using the “mgd77togmt” utility. NBP1701.gmt can be used with the GMT plotting package.

The data used to produce the NBP1701.mgd file can be found on the distribution media in the file /process/NBP1701proc.tar. The data files in the archive contain a day’s data and follow the naming convention Dddd.fnl.tz, where ddd is the year-day. These files follow a space-delimited columnar format that may be more accessible for some purposes. They contain data at one-second intervals rather than one minute and are individually “gzipped” to save space. Below is a detailed description of the MGD77 data set format. The other files in the archive contain interim processing files and are included to simplify possible reprocessing of the data using the RVDAS NBP processing scripts.

All decimal points are implied. Leading zeros and blanks are equivalent. Unknown or unused fields are filled with 9’s. All “corrections”, such as time zone, diurnal magnetics, and EOTVOS, are understood to be added.

Col	Len	Type	Contents	Description, Possible Values, Notes
1	1	int	Data record type	Set to "5" for data record
2-9	8	char	Survey identifier	
10-12	3	int	Time zone correction	corrects time (in chars 13-27) to UTC when added; 0=UTC
13-16	4	int	Year	4 digit year
17-18	2	int	Month	2 digit month
19-20	2	int	Day	2 digit day
21-22	2	int	Hour	2 digit hour
23-27	5	real	Minutes x 1000	
28-35	8	real	Latitude x 100000	Positive = North, Negative = South. (-9000000 to 9000000)
36-44	9	real	Longitude x 100000	Positive = East, Negative = West. (-18000000 to 18000000)
45	1	int	Position type code	1 = Observed fix, 3 = Interpolated, 9 = Unspecified
46-51	6	real	Bathymetry, 2-way travel time	In 10,000th of seconds. Corrected for transducer depth and other such corrections.
52-57	6	real	Bathymetric, corrected depth	In tenths of meters
58-59	2	int	Bathymetric correction code	This code details the procedure used for determining the sound velocity correction to depth
60	1	int	Bathymetric type code	1 = Observed, 3 = Interpolated (Header Seq. 12), 9 = Unspecified
61-66	6	real	Magnetics total field, 1 <sup>st</sup> sensor	In tenths of nanoteslas (gammas)
67-72	6	real	Magnetics total field, 2 <sup>nd</sup> sensor	In tenths of nanoteslas (gammas), for trailing sensor
73-78	6	real	Magnetics residual field	In tenths of nanoteslas (gammas). The reference field used is in Header Seq. 13
79	1	int	Sensor for residual field	1 = 1 <sup>st</sup> or leading sensor, 2 = 2 <sup>nd</sup> or trailing sensor, 9 = Unspecified
80-84	5	real	Magnetics diurnal correction	In tenths of nanoteslas (gammas). (In nanoteslas) if 9-filled (i.e., set to "+9999"), total and residual fields are assumed to be uncorrected; if used, total and residual are assumed to have been already corrected.
85-90	6	F6.0	Depth or altitude of magnetics sensor	(In meters). Positive = Below sea level, 3 = Above sea level
91-97	7	real	Observed gravity	In 10 <sup>th</sup> of mgals. Corrected for Eotvos, drift, tares
98-103	6	real	EOTVOS correction	In 10 <sup>th</sup> of mgals. $E = 7.5 V \cos \phi \sin \alpha + 0.0042 V^2$
104-108	5	real	Free-air anomaly	In 10 <sup>th</sup> of mgals, G = observed, G = theoretical
109-113	5	char	Seismic line number	Cross reference for seismic data
114-119	6	char	Seismic shot-point number	
120	1	int	Quality code for navigation	5 = Suspected, by the originating institution 6 = Suspected, by the data center 9 = No identifiable problem found

## Science of Opportunity

### ADCP

The shipboard ADCP system measures currents in a depth range from about 30 to 300 m -- in good weather. In bad weather or in ice, the range is reduced, and sometimes no valid measurements are made. ADCP data collection is the OPP-funded project of Eric Firing (University of Hawaii) and Teri Chereskin (Scripps Institution of Oceanography). Data is collected on both the LMG and the NBP for the benefit of scientists on individual cruises, and for the long-term goal of building a profile of current structure in the Southern Ocean.

### pCO<sub>2</sub>

The NBP carries a pCO<sub>2</sub> measurement system from Lamont-Doherty Earth Observatory (LDEO). pCO<sub>2</sub> data is recorded by RVDAS and transmitted to LDEO at the end of each cruise. You will find pCO<sub>2</sub> data in a file named NBP1701pco2.tar in the /process directory, which contains the pCO<sub>2</sub> instrument's data merged with GPS, meteorological and other oceanographic measurements. For more information contact Colm Sweeney ([csweeney@ldeo.columbia.edu](mailto:csweeney@ldeo.columbia.edu)).

## Cruise Science

### CTD

The CTD data has been placed in the tar file /ocean/NBP1701ctd.tar. The archive contains tar files NBP1701proc.tar.

### XBT

During a cruise, eXpendable BathyThermographs (XBTs) may have been used to obtain water column temperature profiles, providing corrections to the sound velocity profile for the multibeam system. The data files from those launches would be included as NBP1701xbt.tar in the /ocean directory. **No XBTs were collected on this cruise.**

### RVDAS

The Research Vessel Data Acquisition System (RVDAS) was developed at Lamont-Doherty Earth Observatory of Columbia University and has been in use on its research ship for many years. It has been extensively adapted for use on the USAP research vessels.

Daily data processing of the RVDAS data is performed to calibrate and convert values into useable units and as a quality-control on operation of the DAS. Raw and processed data sets from RVDAS are included in the data distribution. The tables below provide detailed information on the sensors and data. Be sure to read the “Significant Acquisition Events” section for important information about data acquisition during this cruise.

## Sensors and Instruments

RVDAS data is divided into two general categories, *underway and navigation*. They can be found on the distribution media as subdirectories under the top level rvdas directory: /rvdas/uw, and /rvdas/nav. Processed oceanographic data is in the top level directory, /process. Each instrument or sensor produces a data file named with its channel ID. Each data file is g-zipped to save space on the distribution media. Not all data types are collected every day or on every cruise.

The naming convention for data files produced by the sensors and instruments is

NBP[CruiseID][ChannelID].dDDD

Example:      NBP1701mwx1.d025

- The CruiseID is the numeric name of the cruise, in this case, NBP1701.
- The ChannelID is a 4-character code representing the system being logged. An example is “mwx1,” the designation for meteorology.
- DDD is the day of year the data was collected

## Underway Sensors

### Meteorology and Radiometry

Measurement	String ID	Collection Status	Rate	Instrument
Air Temperature	mxw1 (met)	Continuous	1/sec	RM Young 41372LC
Relative Humidity	mxw1 (met)	Continuous	1/sec	RM Young 41372LC
Wind Speed / Direction	mxw1 (pus,sus)	Continuous	1/sec	Gill Instruments 1390-PK-062
Barometer	mxw1 (met)	Continuous	1/sec	RM Young 61201
PAR	mxw1 (met)	Continuous	1/sec	Biospherical Instruments QSR-240
PIR	mxw1 (met)	Continuous	1/sec	Eppley PIR
PSP	mxw1 (met)	Continuous	1/sec	Eppley PSP
GUV	pguv	Continuous	2/sec	Biospherical Instruments GUV-2511

### Geophysics

Measurement	String ID	Collection Status	Rate	Instrument
Gravimeter	grv1	Continuous	1/sec	BGM3/210
Bathymetry	knud	Continuous	varies	Knudsen Chirp
Bathymetry	mbdp	Continuous	varies	Kongsberg EM122

### Oceanography

Measurement	String ID	Collection Status	Rate	Instrument
Conductivity	tsg1,tsg2	Continuous	0.5/sec	Sea-Bird SBE 45
Ocean Surface Temperature	rtmp	Continuous	1.2/sec	Sea-Bird SBE 38
Transmissometer	hdas	Continuous	0.5/sec	WetLabs C-Star
Fluorometer	hdas	Continuous	0.5/sec	WetLabs AFLT
pCO <sub>2</sub>	pco2	Continuous	0.017/sec	LDEO instrumentation
ADCP	adcp	Continuous	1/sec	UHDAS
Bathymetry	sim1	Continuous	varies	Simrad EK60 Sonar

### Navigational Instruments

Measurement	String ID	Collection Status	Rate	Instrument
Heading, Speed, Course, GPS, Heave, Roll and Pitch	s330	Continuous	1/sec	Seapath 330 GPS
Heading, Speed, Course, GPS, Heave, Roll and Pitch	seap	Continuous	1/sec	Seapath 200 GPS
Heading, Speed, Course, and GPS	PCOD	Continuous	1/sec	Furuno GP-330B
Heading	gyr1	Continuous	0.2/sec	Yokogawa Compass

## Data

Data is received from the RVDAS system via RS-232 serial connections. A time tag is added at the beginning of each line of data in the form,

```
yy+dd:hh:mm:ss.sss [data stream from instrument]
```

where

yy	= two-digit year
ddd	= day of year
hh	= 2 digit hour of the day
mm	= 2 digit minute
ss.sss	= seconds

All times are reported in UTC.

The delimiters that separate fields in the raw data files are often spaces and commas but can be other characters such as : = @. Occasionally no delimiter is present. Care should be taken when reprocessing the data that the field's separations are clearly understood.

In the sections below a sample data string is shown, followed by a table that lists the data contained in the string.

*Each section on the next page describes a type of data file (file name extension in parentheses) followed by a typical line of data in the file. In the table(s) for each section is a description of the fields within each line of data. Note: most data files listed below will be included with each cruise's data distribution; however some types of files may be omitted if the instrument was not operating during the cruise. The available data files can be found in the /rvdas/uw and /rvdas/nav directories on the distribution disc.*

**Underway Data** /rvdas/uw**Sound Velocity Probe (svp1)**

15+055:20:27:24.018 1535.43

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	Sound Velocity, from ADCP sonar well	xxxx.xx	m/s

**Meteorology (mwx1)****MET**

15+055:20:27:24.636 MET,12.1,-39,-6.07,77.4,178.0729,0.809536,-0.1235019,268.1754,267.9648,970.7878

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	MET Flag		
3	Power Supply Voltage	vv.v	V
4	Enclosure Relative Humidity (not implemented)	xx.x	%
5	Air Temperature, Celsius	xx.x	C
6	Air Relative Humidity	xx.x	%
7	PAR (Photosynthetically Available Radiation)	xxx.xxxx	mV
8	PSP (Shortwave Radiation)	x.xxxxxx	mV
9	PIR Thermopile (Longwave Radiation)	x.xxxxxx	mV
10	PIR Case Temperature	xxx.xxxx	K
11	PIR Dome Temperature	xxx.xxxx	K
12	Barometer	xxx.xxxx	mBar

**PUS**

15+055:21:47:42.452 PUS,A,037,014.36,M,+325.38,-010.29,60,0F

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	PUS Flag		
3	A	x	A
4	Port Wind Relative Direction	xxx	degrees
5	Port Wind Relative Speed	xxx.xx	m/s
6	M = Meters (for previous)	x	M
7	Sound Speed	xxx.xx	m/s
8	Sonic Temperature	xxx.xx	C
9	Unit Status*	xx	numeric
10	Checksum	xx	alphanumeric

**Status**

00 = Good, 60 = Good. Any other value indicates fault

**SUS**

15+055:21:50:48.409 SUS,A,338,012.63,M,+326.15,-009.05,60,0F

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	SUS Flag		
3	A	x	A
4	Starboard Wind Relative Direction	xxx	degrees
5	Starboard Wind Relative Speed	xxx.xx	m/s
6	M = Meters (for previous)	x	M
7	Sound Speed	xxx.xx	m/s
8	Sonic Temperature	xxx.xx	C
9	Unit Status*	xx	numeric
10	Checksum	xx	alphanumeric

**Status**

00 = Good, 60 = Good. Any other value indicates fault

**Knudsen (knud)**

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	3.5kHz = Low frequency in use	x.xxxx	3.5kHz
3	Low Frequency Depth	xxxx.xx	m
4	Valid Flag	x	0
5	12.0kHz = High frequency in use	xx.xxxx	12.0kHz
6	High Frequency Depth	xxxx.xx	m
7	Valid Flag	x	0
8	Sound Speed Velocity	xxxx	m/s
9	Latitude	xx.xxxxxx	degrees
10	Longitude	xx.xxxxxx	degrees

**Gravimeter (grv1)**

15+056:14:21:21.153 01:025268 00

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	01:	xx:	01
3	Gravity Count*	xxxxxx	Flit Count
4	Error Flag	xx	numeric

**Error Flag**

00 = All well, 01 = CPS malfunction, 02 = Sensor Malfunction, 03 = CPS and sensor Malfunction

A gravity tie is taken at the start of the cruise and applied throughout the cruise. There is no accounting for drift after the pre-cruise gravity time. The post cruise gravity tie is available by requesting it from ethq@usap.gov.



**pCO<sub>2</sub> (pco2)**

15+056:14:41:10.392 2015056.60236 2608.36 30.14 977.91 48.25 368.76 353.92 -1.18 -1.26 0.00 Equil

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	pCO <sub>2</sub> time tag*	yyyyddd.ttt	UTC
3	Raw Voltage (IR)	xxxx.xx	mV
4	Cell Temperature	xx.xx	C
5	Equilibration Pressure	xxx.xx	mBar
6	Flowrate	xxx.xx	cm <sup>3</sup> /min
7	pCO <sub>2</sub> Pressure	xxx.xx	μAtm
8	VCO <sub>2</sub> Concentration	xx.xx	ppm
9	Equilibrator Temperature, RTD	xx.xx	C
10	Equilibrator Temperature, SBE38	xx.xx	C
11	Valve Position	xx	numeric
12	Flow Source*		text

**pCO<sub>2</sub> time tag**

ttt = fractional time of day

**Flow Source**Equil = pCO<sub>2</sub> Measurement**Micro TSG (tsg1, tsg2)**

15+056:15:06:06.644 -1.1809, 2.73404, 34.0574, 1442.367

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	Temperature	xx.xxxx	C
3	Conductivity	xx.xxxx	s/m
4	Salinity	xx.xxxx	PSU
5	Sound Velocity	xxxx.xxx	m/s

**Remote Temperature (rtmp)**

15+056:15:10:38.244 -1.4644

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	Temperature, Seawater Intake	xx.xxxx	C

**GUV (pguv)**

15+057:14:51:33.808 022615 065133 .000132 .010878 .047479 .004407 -.002799 .014652 .027558 .094395  
 .417814 -4.466095

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	Date	mmddyy	UTC-4
3	Time	hhmmss	UTC-4
4	Ed0GND (sensor ground voltage)	xxxxxx	V
5	Ed0320 (downwelling 320nm irradiance)	xxxxxx	μW
6	Ed0340 (downwelling 340nm irradiance)	xxxxxx	μW
7	Ed0313 (downwelling 313nm irradiance)	xxxxxx	μW
8	Ed0305 (downwelling 305nm irradiance)	xxxxxx	μW
9	Ed0380 (downwelling 380nm irradiance)	xxxxxx	μW
10	Ed0PAR (downwelling 400-700nm irradiance)	xxxxxx	μE
11	Ed0395 (downwelling 395nm irradiance)	xxxxxx	μW
12	Ed0Temp (sensor array temperature)	xxxxxx	C
13	Ed0Vin (input voltage)	x.xxxxxx	V

**Engineering (eng1)**

15+057:16:41:24.536 12.25 23.21 507.8 0.6 162.6 -751.9 0 0 NAN NAN -10.3 7.2

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	Supply Voltage	xx.xx	V
3	Case Temperature	xx.xx	C
4	Seawater Flow, Aquarium Room	xxx.x	l / min
5	Seawater Flow, Helo-deck	x.x	l / min
6	Seawater Flow, Hydro-lab	xxx.x	l / min
7	Seismic Air Pressure	xxx.x	lbf/in <sup>2</sup>
8	Not Currently Hooked Up	x	0 or NAN
9	Not Currently Hooked Up	x	0 or NAN
10	Not Currently Hooked Up	x	0 or NAN
11	Not Currently Hooked Up	x	0 or NAN
12	Altimeter for Yo-Yo Camera - <b>Rarely used*</b>	xx.xx	m
13	Transmissometer for Yo-Yo camera - <b>Rarely used*</b>	xxx.x	%

**Altimeter**

This is rarely used, and only provides real data when connected. When not connected, provides a value approx = -10.

**Transmissometer**

This is rarely used, and only provides real data when connected. When not connected, provides a value range of approx = 0 to 10.

**Hydro DAS (hdas)**

15+057:16:07:09.456 12.15038 12.39402 336.5517 4431.724 -1 20.5 64 33.5 43.5

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	Supply Voltage	xx.xxxxx	V
3	Case Temperature	xx.xxxxx	C
4	Fluorometer	xxx.xxxx	mV
5	Transmissometer	xxxx.xxx	mV
6	Sea Water Valve*	x	-1 or 0
7	Flow Meter 1 Frequency	xx.x	Hz
8	Flow Meter 2 Frequency	xx.x	Hz
9	Flow Meter 3 Frequency	xx.x	Hz
10	Flow Meter 4 Frequency	xx.x	Hz

**Sea Water Valve**

-1 = Stern Thruster Valve, 0 = Moon Pool Valve

**Winch (bwnc, cwnc, twnc)**

15+057:14:12:24.405 02RD,2015-02-26T14:55:32.051,STBD TRAWL,00000064,-00000.0,-00023.2,3594

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	LAN ID		alphanumeric
3	LCI-90i Date and Time	yyyy-mm-ddThh:mm:ss.sss	
4	Winch Name		alphabetical
5	Tension	xxxxxxxxx	lbs
6	Speed	xxxxx.x	m/min
7	Payout	xxxxx.x	m
8	Checksum	x.xxxx	numeric

**Multibeam (mbdp)**

15+058:22:04:52.826 \$KIDPT,594.68,7.67,12000.0\*43

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	KIDPT	x.x	m
3	Depth at Transducer	x.x	m
4	Distance to Waterline from Transducer	x.x	m
5	Maximum Range in Use	x.x	alphanumeric
6	Checksum	xx	UTC

**Navigational Data** */rvdas/nav***GPS (s330, seap, PCOD)**

1. ***Seapath 330***
  - a. NMEA 0183 strings
    - i. GPZDA
    - ii. GPGGA
    - iii. GPVTG
    - iv. GPHDT
    - v. GPRMC
  - b. Proprietary Strings
    - i. PSXN 20
    - ii. PSXN 22
    - iii. PSXN 23
2. ***Seapath 200***
  - a. NMEA 0182 strings
    - i. GPZDA
    - ii. GPGGA
    - iii. GPVTG
    - iv. GPHDT
  - b. Proprietary Strings
    - i. PSXN 20
    - ii. PSXN 22
    - iii. PSXN 23
3. ***Furuno GP-330B***
  - a. NMEA 0183 strings
    - i. GPZDA
    - ii. GPGGA
    - iii. GPVTG
    - iv. GPRMC
    - v. GPGLL
    - vi. GPDTM

**GPZDA**

15+051:21:02:04.507 \$GPZDA,210204.39,20,02,2015,,\*6F

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$GPZDA		
3	Time	hhmmss.ss	UTC
4	Day	dd	UTC
5	Month	mm	UTC
6	Year	yyyy	UTC
7	(empty field)	x	Blank or 0
8	Checksum	xx	alphanumeric

**GPGBA**

15+051:21:02:02.507 \$GPGBA,210202.38,7712.979244,S,16741.040258,W,1,12,0.7,-5.04,M,-55.90,M,,\*6F

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$GPGBA		
3	Time	hhmmss.ss	UTC
4	Latitude	ddmm.mmmmmm	degrees
5	North or South (for previous)	x	N or S
6	Longitude	ddmm.mmmmmm	degrees
7	East or West (for previous)	x	E or W
8	GPS quality indicator*	x	0,1,2,3,4,5, or 6
9	Number of satellites in use (00-99)	xx	00-99
10	HDOP	x.x	
11	Antenna height	x.xx	m
12	M = Meters (for previous)	x	M
13	Geoidal height	x.xx	m
14	M = Meters (for previous)	x	M
15	Age of DGPS corrections (seconds)	x.x	seconds
16	Station ID of DGPS (if used)	x	numeric
17	Checksum	xx	alphanumeric

**Quality**

0 = invalid, 1 = GPS SPS, 2 = DGPS, 3 = PPS, 4 = RTK, 5 = float RTK, 6 = dead reckoning

**GPVTG**

15+051:16:47:06.625 \$GPVTG,357.84,T,251.99,M,9.5,N,17.7,K,A\*15

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$GPVTG		
3	Heading	x.xx	degrees
4	T = True (for previous)	x	T
5	Heading	x.xx	degrees
6	M = Magnetic (for previous)	x	M
7	Speed over Ground (knots)	x.x	knots
8	N = knots (for previous)	x	N
9	Speed over Ground (kilometers per hour)	x.x	km/h
10	K = km per hour (for previous)	x	K
11	Mode*	X	A,D,E, or N
12	Checksum	xx	alphanumeric

**Modes**

A = GPS used, D = DGPS used, E = Dead reckoning used, N = Invalid position / velocity

**GPRMC**

15+051:21:02:04.741 \$GPRMC,210204.38,A,7712.979182,S,16741.063669,W,9.4,270.82,200215,105.6,E,A\*06

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$GPRMC		
3	Time	hhmmss.sss	UTC
4	Status*	x	A or N
5	Latitude	ddmm.mmmmmm	degrees
6	North or South (for previous)	x	N or S
7	Longitude	ddmm.mmmmmm	degrees
8	East or West (for previous)	x	E or W
9	Speed over Ground, True	x.x	knots
10	Course over Ground True	x.xx	degrees
11	Date	ddmmyy	UTC
12	Magnetic Variation	x.x	degrees
13	East or West (for previous)	x	E or W
14	Mode*	x	alphanumeric
15	Checksum	xx	UTC

**GPHT**

15+051:21:02:04.741 \$GPHT,268.87,T\*06

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$GPHT		
3	Heading, True	x.xx	degrees
4	T = True (for previous)	x	T
5	Checksum	xx	alphanumeric

**GPGLL**

16+077:00:00:00.725 \$GPGLL,6356.6505,S,05716.0002,W,000000,A,A\*4F

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$GPGLL		
3	Latitude	ddmm.mmmmmm	degrees
4	North or South (for previous)	x	N or S
5	Longitude	ddmm.mmmmmm	degrees
6	East or West (for previous)	x	E or W
7	Time of Position (not received)	hhmmss.ss	UTC
8	Status*	x	A or V
9	Mode*	x	alphanumeric
10	Checksum	xx	alphanumeric

**Status**

A = Data Valid, V = Data not valid

**Modes**

A = GPS used, D = DGPS used, E = Dead reckoning used, M = Manual input mode, S = Simulator Mode, N = Invalid position / velocity

**GPDTM**

16+077:00:00:02.527 \$GPDTM,W84,,0000.0000,N,00000.0000,E,0.0,W84\*5F

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$GPDTM		
3	Local Datum Code*	XXX	alphanumeric
4	Local datum subdivision code	x	numeric
6	Lat offset	x	alphanumeric
7	North or South (for previous)	x	N or S
8	Lon offset	x	alphanumeric
9	East or West (for previous)	x	E or W
10	Altitude offset, meters	x,x	numeric
11	Reference datum code*	xxx	alphanumeric
12	Checksum	xx	alphanumeric

**Datum Codes**

W84 = WGS84, W72 = WGS72, S85 = SGS85, P90 = PE90, 999 = User defined

**PSXN 20**

15+051:22:20:58.740 \$PSXN,20,1,0,0,0\*3A

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$PSXN		
3	20		
4	Horizontal position and velocity quality*	x	0,1,2
5	Height and vertical velocity quality*	x	0,1,2
6	Heading quality*	x	0,1,2
7	Roll and pitch quality*	x	0,1,2
8	Checksum	xx	alphanumeric

**Qualities**

0 = Normal, 1 = Reduced Performance, 2 = Invalid data

**PSXN 22**

15+051:22:20:59.019 \$PSXN,22,0.43,0.50\*3B

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$PSXN		
3	22		
4	Gyro calibration value since system startup	x.xx	degrees
5	Short-term gyro offset	x.xx	degrees
6	Checksum	xx	alphanumeric



**PSXN 23**

15+051:22:20:58.748 \$PSXN,23,-0.20,-0.09,279.85,0.24\*34

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$PSXN		
3	23		
4	Roll, port side up is positive	x.xx	degrees
5	Pitch, bow up is positive	x.xx	degrees
6	Heading, True	x.xx	degrees
7	Heave, positive is down	x.xx	m
8	Checksum	xx	alphanumeric

**Gyro Compass (gyr1)**

15+055:20:27:23.653 \$HEHDT,087.31,T\*12

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$HEHDT		
3	Heading	x.xx	degrees
4	T = True (for previous)	x	T
5	Checksum	xx	alphanumeric

**Processed Data** /process**pCO<sub>2</sub> – Merged**

15+055:11:24:43.960 2015055.46596 2534.72 32.41 975.33 48.86 356.94 341.67 -1.20 -1.27 0.00 Equil -  
 75.9209 178.9696 -1.435 33.852 2.26 7.86 137.38 975.34 163.80 9.31 253.75 NaN -1.27 33.84 -1.14 -  
 1.0

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	pCO <sub>2</sub> time tag*	yyyyddd.ttt	UTC
3	Raw Voltage (IR)	xxxx.xx	mV
4	Cell Temperature	xx.xx	C
5	Equilibration Pressure	xxx.xx	mBar
6	Flowrate	xxx.xx	cm <sup>3</sup> /min
7	pCO <sub>2</sub> Pressure	xxx.xx	μAtm
8	VCO <sub>2</sub> Concentration	xx.xx	ppm
9	Equilibrator Temperature, RTD	xx.xx	C
10	Equilibrator Temperature, SBE38	xx.xx	C
11	Valve Position	xx	numeric
12	Flow Source*		text
13	Latitude	xx.xxxxx	degrees
14	Longitude	xxx.xxxxx	degrees
15	Sea Water Intake Temperature	xx.xxx	C
16	Sea Surface Salinity	xx.xxx	PSU
17	Sea Surface Fluorometry	x.xxx	mg/m <sup>3</sup>
18	True Wind Speed	x.xx	m/s
19	True Wind Direction	x.xx	degrees
20	Barometric Pressure	xxx.xx	mBar
21	Hydro-Lab H <sub>2</sub> O Flow Rate	xxx.x	l / min
22	Speed over Ground	x.xx	knots
23	Course Made Good	xx.xx	degrees
24	Unused		
25	TSG2 Temperature	x.xx	C
26	TSG2 Salinity	xx.xx	PSU
27	TSG1 Temperature	x.xx	C
28	Sea Water Valve*	x	-1 or 0

**pCO<sub>2</sub> time tag**

ttt = fractional time of day

**Flow Source**

Equil = pCO<sub>2</sub> Measurement

**Sea Water Valve**

-1 = Stern Thruster Valve, 0 = Moon Pool Valve

## Calculations

### PAR

Coefficients `parc1` and `parcv` for this cruise can be found in the `instrument.coeff` file as the variable labeled PAR, respectively. Variable `par` is the raw data in mV, as described in the “mw1” file description. The calibration scale and probe offset dark are values taken from the PAR Cal Sheet.

```
par = raw data mV
calibration scale = 5.8644 V/(μEinstiens/cm2sec)
parc1 = 1 / scale = .17
probe offset dark = -.1 mV
parcv = dark x 1000 mV/V = -0.0001 V
((par / 1000 mV/V) - parcv) x parc1 x 10000 cm2/m2 = μEinstiens/m2sec
```

Calculations (extracted from the C code):

```
/* Convert from mV to V */
par /= 1000;
/* (par V - vdark V) / Calibration Scale Factor V/uE/cm2sec */
parCalc = (par - parcv) * parc1 * 10000;
```

### PSP

Coefficient `pspCoeff` for this cruise can be found in the `instrument.coeff` file as the variable labeled PSP1. Variable `psp` is the raw data in mV, as described in the “mw1” file description.

```
psp = raw data mV
calibration scale = pspCoeff x 10^-6 V/(W/m2)
psp / (scale x 1000 mV/V) = W/m2
```

Calculations (extracted from the C code):

```
/* Convert from mV to W/m^2 */
pspCalc = (psp * 1000 / pspCoeff);
```

## PIR

Coefficient `pirCoeff` for this cruise can be found in the `instrument.coeff` file as the variable labeled PIR1. Variable `pir_thermo` is the raw data in mV, `pir_case` is the PIR case temperature in Kelvins and `pir_dome` is the PIR dome temperature in Kelvins, as described in the “mwx1” file description. Hard-coded “C” coefficients are shown below:

```
Dome constant = 3.5
```

```
Sigma = 5.6704e-8
```

```
pir_thermo = raw data mV
```

```
calibration scale = pirCoeff x 10-6 V/(W/m2)
```

```
pir_thermo / (scale x 1000 mV/V) = W/m2
```

Calculations (extracted from the C code):

```
/* convert mV to W/m^2 */  
pirCalc = (pir_thermo * 1000 / pirCoeff)  
/* correct for case temperature */  
pirCalc += sigma * pow(pir_case,4)  
/* correct for dome temperature */  
pirCalc -= 3.5 * sigma * (pow(pir_dome, 4) - pow(pir_case, 4))
```

## Acquisition Problems and Events

This section lists problems with acquisition noted during this cruise including instrument failures, data acquisition system failures and any other factor affecting this data set. The format is ddd:hh:mm (ddd is year-day, hh is hour, and mm is minute). Times are reported in UTC.

Start	End	Description
360:12:18		Data collection begins. -52 37.171, -74 47.959
361:17:30		MB Logging Start -55 55, -71 28
362:18:40		Reboot MOXA for Maintenance
362		Exit Chilean EEZ
363:04:00		Reboot MOXA for Maintenance
365:11:05		EM122 1PPS error – Reboot of EM122
366:17:05		Arrive Rothera – DAS off
366:21:00		Depart Rothera – DAS on
	017:17:45	Data collection completes -77 09, 166 13

## Appendix A: Sensors

### NBP1701 Sensors

Sensor	Description	Serial	Last Cal Date	Comments
<b>Meteorology and Radiometry</b>				
Port Anemometer	Gill Instruments 1390-PK-062	924057	11/18/2009	
Stbd Anemometer	Gill Instruments 1390-PK-062	847014	9/29/2010	
Bridge Anemometer	RM Young 5106	WM128975	10/27/2011	ECO Use
Barometer	RM Young 61201	00872	5/20/2015	
Temperature / Humidity	RM Young 41372LC	06135	7/10/2015	
PIR	Eppley PIR	3284SF3	1/13/2016	
PSP	Eppley PSP	32850F3	1/15/2016	
PAR (Mast)	Biospherical Instruments QSR-240	6357	2/17/2015	
GUV (Mast)	Biospherical Instruments GUV-2511	25110203114	7/20/2016	

Sensor	Description	Serial	Last Cal Date	Comments
<b>Underway Seawater Sampling System</b>				
Micro-TSG	Sea-Bird SBE 45	4546167-0199	2/19/2016	Primary
Micro-TSG	Sea-Bird SBE 45	4549120-0226	5/27/2015	Secondary
Digital Remote Temp	Sea-Bird SBE 38	3850449-0389	6/8/2015	
Transmissometer	WetLabs C-Star	CST-889DR	7/6/2015	
Fluorometer	WetLabs AFLT	FLRTD-4158	10/23/2015	

Sensor	Description	Serial	Last Cal Date	Comments
<b>CTD</b>				
Altimeter	Valeport VA-500	51519	7/10/2015	
Carousel Water Sampler	Sea-Bird SBE 32	3270675-0925	NA	
SBE 11+ Deck Unit	Sea-Bird SBE 11+	11P19858-0490	NA	
Conductivity (Primary)	Sea-Bird 4C 6800m	041852	11/25/2015	
Conductivity (Secondary)	Sea-Bird 4C 6800m	044151	6/30/2015	
Transmissometer	WetLabs C-Star	CST-557DR	7/27/2015	
Fluorometer	WetLabs FLRTD	FLRTD-0397	2/23/2045	
CTD Fish	Sea-Bird SBE 9+	09P70675-1130	2/5/2016	
CTD Pressure Sensor	Sea-Bird SBE 9+	120089	1/27/2016	
Dissolved Oxygen	Sea-Bird SBE 43	0080	1/20/2016	Primary
Dissolved Oxygen	Sea-Bird SBE 43	0082	3/25/2016	Secondary
CTD Pump 1	Sea-Bird 5T, PN 90160	051646 3.0K	10/9/2014	Primary
CTD Pump 2	Sea-Bird 5T, PN 90543	055644 3.0K	10/9/2014	Secondary
Surface PAR	QSR-240	6357	2/17/2015	Fed to CTD, on Mast
PAR	Biospherical Instruments QSP-200L4S	4361	2/18/2015	
Temperature	Sea-Bird 03-02/F	031541	11/26/2015	Primary
Temperature	Sea-Bird 3F 6800m	03P5185	6/30/2015	Secondary
Transmissometer	WetLabs C-Star	CST-557DR	7/27/2015	

## Appendix B: Calibration Sheets

### Gravity

#### BGM3 ship-to-shore gravity tie report

S. Blackman / A. Scott, vessel: R/V Palmer

Release Date: 2016/10/18 19:52:08 UTC

Sensor: S210

Software version: 1.2

Port/Pier/Berth: Pratt Pier

Gravity station number	9337-50 (3)
Station name	Harbour Admin Bldg
mGal at pier	981320.82
Tie start time UTC	2016/10/18 19:10:36.961
Samples used	3600
Land tie used	Yes
Water height to pier 1	10 ft 6 in
Water height to pier 2	10 ft 9 in
Water height to pier 3	11 ft 0 in
Average of filtered counts	25195.216448472
Filter length	361
Scale factor	4.994070552
<b>NEW BIAS</b>	<b>855495.14</b>

Table 1: Gravity tie information

## Meteorology

### Anemometers

Cal sheet not required



## Barometer



**R.M. Young Company**  
2801 Aero Park Drive  
Traverse City, Michigan 49686 USA

### CALIBRATION REPORT Barometric Pressure

Customer: *Lockheed Martin Corp*

Test Number: 5520-01B

Customer PO: 4100959204

Test Date: 20 May 2015

Sales Order: 4756

Test Sensor:

Model: 61201

Serial Number: BP00872

Description: Barometric Pressure Sensor

Report of calibration comparison of test barometric pressure sensor with National Institute of Standards and Technology traceable standard pressure calibrator at five pressures in the R.M. Young Company controlled pressure facility. Calibration accuracy  $\pm 1.0$  hPa.

Reference Pressure (hPa)	Voltage Output (millivolts)	Indicated (1) Pressure (hPa)
800.0	0	800.0
875.0	1252	875.1
950.0	2501	950.1
1025.0	3750	1025.0
1100.0	4997	1099.8

(1) Calculated from voltage output

All reference equipment used in this calibration procedure have been tested by comparison to traceable standards certified by the National Institute of Standards and Technology.

Reference Instrument

Druck Pressure Controller Model DPI515  
Fluke Multimeter Model 8060A

Serial # NIST Test Reference

51500497 0046591  
4865407 8604897

Tested By: \_\_\_\_\_

**METEOROLOGICAL INSTRUMENTS**  
Tel: 231-946-3980 Fax: 231-946-4772 Email: met.sales@youngusa.com Website: youngusa.com  
ISO 9001:2008 CERTIFIED

## Temperature / Humidity



**R.M. Young Company**  
2801 Aero Park Drive  
Troy, Michigan 48068 USA

**CALIBRATION REPORT****Temperature**

Customer: *Lockheed Martin Corp*

Test Number: 5710-04T

Test Date: 10 July 2015

Customer PO: 45000063237

Sales Order: 4867

**Test Sensor:**

Model: 41372LC

Serial Number: TS06135

Description: Temperature/Relative Humidity Sensor

Report of calibration comparison of test temperature sensor with National Institute of Standards and Technology traceable standard thermometers at three temperatures in the R.M. Young Company controlled temperature calibration bath facilities. Calibration accuracy  $\pm 0.1^\circ$  Celsius.

Bath Temperature (degrees C)	Current Output (milliamps)	Indicated (1) Temperature (degrees C)
-49.85	4.023	-49.86
-0.01	11.996	-0.03
49.97	19.993	49.96

(1) Calculated from current output

All reference equipment used in this calibration procedure have been tested by comparison to traceable standards certified by the National Institute of Standards and Technology.

Reference Instrument	Serial #	NIST Test Reference
Brooklyn Thermometer Model 43-FC	3006-118	W204690
Brooklyn Thermometer Model 22332-D5-FC	25071	W204691
Brooklyn Thermometer Model 2X100-D7-FC	77532	W204692
Keithley Multimeter Model 191	15232	8604897

Tested By: *R. B. Young*

**METEOROLOGICAL INSTRUMENTS**  
Tel: 231-946-3930 Fax: 231-946-4772 Email: met.sales@youngusa.com Website: youngusa.com  
ISO 9001:2008 CERTIFIED

PIR

**THE EPPLEY LABORATORY, INC.**12 Sheffield Avenue, PO Box 419, Newport, Rhode Island USA 02840  
Phone: 401.847.1020 Fax: 401.847.1031 Email: info@eppleylab.com**STANDARDIZATION OF  
EPPLEY PRECISION INFRARED RADIOMETER  
Model PIR**

Serial Number: 32845F3

Resistance: 712  $\Omega$  at 23°C

Temperature Compensation Range: -20° to +40°C

This pyrgeometer has been compared against Eppley's Blackbody Calibration System under radiation intensities of approximately 200 watts meter<sup>-2</sup> and an average ambient temperature of 22°C as measured by Standard Omega Temperature Probe, RTD41.

As a result of a series of comparisons, it has been found to have a sensitivity of:

$$4.18 \times 10^{-6} \text{ volts/watts meter}^{-2}$$

The calculation of this constant is based on the fact that the relationship between radiation intensity and emf is rectilinear to intensities of 700 watts meter<sup>-2</sup>. This radiometer is linear to within  $\pm 1.0\%$  up to this intensity.

The calibration of this instrument is traceable to the International Practical Temperature Scale (IPTS) through a precision low-temperature blackbody.

Eppley recommends a minimum calibration cycle of five (5) years but encourages annual calibrations for highest measurement accuracy. Unless otherwise stated in the remarks section below or on the Sales Order, the results are "AS FOUND / AS LEFT".

Shipped to: NSF/ Lockheed Martin  
Port Hueneme, CA

Date of Test: January 13, 2016

In Charge of Test:

S.O. Number: 64615  
Date: January 14, 2016

Reviewed by:

Remarks:

*End of Report*

## PSP

**THE EPPLEY LABORATORY, INC.**

12 Sheffield Avenue, PO Box 419, Newport, Rhode Island USA 02840  
Phone: 401.847.1020 Fax: 401.847.1031 Email: info@eppleylab.com

**Calibration Certificate**

---

**Instrument:** Precision Spectral Pyranometer, Model PSP, Serial Number 32850F3

**Procedure:** This pyranometer was compared in Eppley's Integrating Hemisphere according to procedures described in *ISO 9847 Section 5.3.1* and Technical Procedure, TP01 of The Eppley Laboratory, Inc.'s Quality Assurance Manual on Calibrations.

**Transfer Standard:** Eppley Standard Precision Pyranometer, Model SPP, Serial Number 37501F3

**Results:**  
**Sensitivity:**  $S = 6.91 \mu\text{V} / \text{Wm}^{-2}$   
**Uncertainty:**  $U_{95} = \pm 0.91\%$  (95% confidence level,  $k=2$ )  
**Resistance:** 706  $\Omega$  at 23°C

**Date of Test:** January 15, 2016

**Traceability:** This calibration is traceable to the World Radiation Reference (WRR) through comparisons with Eppley's AIIF standard self-calibrating cavity pyrheliometers which participated in the Eleventh International Pyrheliometric Comparisons (IPC XI) at Davos, Switzerland in September-October 2010. Unless otherwise stated in the remarks section below or on the Sales Order, the results of this calibration are "AS FOUND / AS LEFT".

**Due Date:** Eppley recommends a minimum calibration cycle of five (5) years but encourages annual calibrations for highest measurement accuracy.

**Customer:** NSF/Lockheed Martin  
Port Hueneme, CA

**Signatures:**  
In Charge of Test: *Brian L. Hurley*  
Reviewed by: *Thomas D. Kirk*

**Eppley SO:** 64614

**Date of Certificate:** January 15, 2016

**Remarks:** Sensitivity before Repairing Element - 7.62  $\mu\text{V} / \text{Wm}^{-2}$

*End of Report*

## PAR (Mast)

## Biospherical Instruments Inc.

## CALIBRATION CERTIFICATE

Calibration Date	2/17/2015
Model Number	QSR240
Serial Number	6357
Operator	TPC
Standard Lamp	V-033(3/7/12)
Probe Excitation Voltage Range:	6 to 18 VDC(+)
Output Polarity:	Positive

Probe Conditions at Calibration (in air):

Calibration Voltage:	6 VDC(+)
Probe Current:	7.2 mA

Probe Output Voltage:

Probe Illuminated	97.3 mV
Probe Dark	1.0 mV
Probe Net Response	96.3 mV
RG780	1.1 mV

Corrected Lamp Output:

Output In Air (same condition as calibration):

9.342E+15	quanta/cm <sup>2</sup> sec
155,13384	uE/m <sup>2</sup> sec

Calibration Scale Factor:

(To calculate irradiance, divide the net voltage reading in Volts by this value.)

Dry:	1.0304E-17	V/(quanta/cm <sup>2</sup> sec)
	6.2054E-04	V/(uE/m <sup>2</sup> sec)

## Notes:

1. Annual calibration is recommended.
2. Calibration is performed using a Standard of Spectral Irradiance traceable to the National Institute of Standards and Technology (NIST).
3. The collector should be cleaned frequently with alcohol.
4. Calibration was performed with customer cable, when available.

QSR240R 05/24/95

## GUV (Mast)



Biospherical Instruments Inc.

GUV-2511 Calibration Certificate											
System Serial Number		25110203114					Date of Calibration		8/3/2016		
Calibration database		25110203114v9.mdb					Date of Certificate		8/4/2016		
DASSN		0069					Standard of Spectral Irradiance		91453(7/20/16)		
Microprocessor Tag Number		4					Operator		TC		
Monochromatic Channels		Wavelength	Responsivity	ScaleSmall	ScaleMedium	ScaleLarge	OffsetSmall	OffsetMedium	OffsetLarge	Measurement Units	
	Address	[nm]	[Amps per $\mu\text{W}/(\text{cm}^2 \cdot \text{nm})$ ]	[Volts per $\mu\text{W}/(\text{cm}^2 \cdot \text{nm})$ ]	[Volts per $\mu\text{W}/(\text{cm}^2 \cdot \text{nm})$ ]	[Volts per $\mu\text{W}/(\text{cm}^2 \cdot \text{nm})$ ]	[volts]	[volts]	[volts]		
Ed0320	2	320	2.3369E-10	2.3836E-05	6.9638E-03	2.1979E+00	3.4492E-05	3.2554E-05	5.6504E-04	$\mu\text{W}/(\text{cm}^2 \cdot \text{nm})$	
Ed0340	6	340	1.8327E-10	1.8693E-05	5.4614E-03	1.8735E+00	4.2136E-05	4.1875E-05	7.6934E-04	$\mu\text{W}/(\text{cm}^2 \cdot \text{nm})$	
Ed0313	8	313	2.0456E-10	2.0865E-05	6.0958E-03	2.1398E+00	9.1228E-04	9.0624E-04	-1.2773E-03	$\mu\text{W}/(\text{cm}^2 \cdot \text{nm})$	
Ed0305	10	305	1.1339E-11	1.1565E-06	3.3789E-04	1.1614E-01	3.5080E-04	3.5087E-04	1.1382E-03	$\mu\text{W}/(\text{cm}^2 \cdot \text{nm})$	
Ed0380	12	380	8.1708E-11	8.3342E-06	2.4349E-03	7.8097E-01	2.8388E-04	2.7513E-04	-3.8577E-05	$\mu\text{W}/(\text{cm}^2 \cdot \text{nm})$	
Ed0395	18	395	2.8750E-10	2.9325E-05	8.5676E-03	2.7082E+00	3.8212E-04	3.8356E-04	1.4618E-03	$\mu\text{W}/(\text{cm}^2 \cdot \text{nm})$	
Broadband Channels		Wavelength	Responsivity	ScaleSmall	ScaleMedium	ScaleLarge	OffsetSmall	OffsetMedium	OffsetLarge	Measurement Units	
	Address	[nm]	[Amps per $\mu\text{E}/(\text{cm}^2 \cdot \text{s})$ ]	[Volts per $\mu\text{E}/(\text{cm}^2 \cdot \text{s})$ ]	[Volts per $\mu\text{E}/(\text{cm}^2 \cdot \text{s})$ ]	[Volts per $\mu\text{E}/(\text{cm}^2 \cdot \text{s})$ ]	[volts]	[volts]	[volts]		
Ed0PAR	13	400-700	1.7117E-05	1.7459E+00	5.1009E+02	1.8027E+05	5.6671E-04	5.6137E-04	-4.7669E-04	$\mu\text{E}/(\text{cm}^2 \cdot \text{sec})$	
Auxilliary Channels		Address	Wavelength	Responsivity	ScaleS	ScaleM	ScaleL	OffsetS	OffsetM	OffsetL	Measurement Units
Ed0Temp	22	0	1	0.01	0.01	0.01	0	0	0	0	C
Ed0Vin	27	0	1	-0.25	-0.25	-0.25	0	0	0	0	V

© Biospherical Instruments Inc., 5340 Riley Street, San Diego, California 92110 USA. Contact [support@biospherical.com](mailto:support@biospherical.com) for more information.

Calibration Data – Do Not Destroy

page 2 of 2



## Underway Seawater Sampling System

## Micro-TSG 2

## Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0389  
CALIBRATION DATE: 05-Oct-16SBE 45 TEMPERATURE CALIBRATION DATA  
ITS-90 TEMPERATURE SCALE

## COEFFICIENTS:


a0 = 3.090837e-005  
 a1 = 2.658070e-004  
 a2 = -1.844963e-006  
 a3 = 1.332162e-007

BATH TEMP (° C)	INSTRUMENT OUTPUT (counts)	INST TEMP (° C)	RESIDUAL (° C)
1.0000	828418.5	1.0000	-0.0000
4.5000	706628.0	4.5000	0.0000
14.9999	447305.9	14.9999	0.0000
18.5000	386484.7	18.4999	-0.0001
24.0000	309027.4	24.0000	-0.0000
29.0000	253718.2	29.0001	0.0001
32.5000	221745.8	32.4999	-0.0001

n = Instrument Output (counts)

Temperature ITS-90 (°C) =  $1 / \{a_0 + a_1[\ln(n)] + a_2[\ln^2(n)] + a_3[\ln^3(n)]\} - 273.15$ 

Residual (°C) = instrument temperature - bath temperature

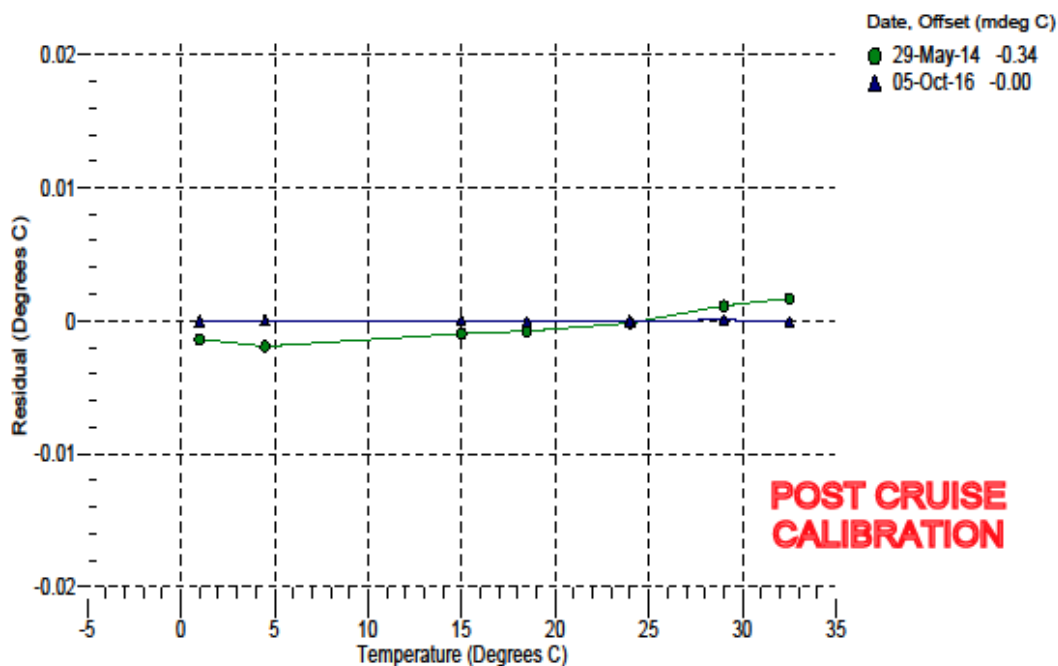

# Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0389  
 CALIBRATION DATE: 05-Oct-16

SBE 45 CONDUCTIVITY CALIBRATION DATA  
 PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

## COEFFICIENTS:

g = -1.011215e+000  
 h = 1.476175e-001  
 i = -8.280491e-004  
 j = 7.730207e-005


CPcor = -9.5700e-008  
 CTcor = 3.2500e-006  
 WBOTC = 1.2700e-007

BATH TEMP (°C)	BATH SAL (PSU)	BATH COND (S/m)	INSTRUMENT OUTPUT (Hz)	INSTRUMENT COND (S/m)	RESIDUAL (S/m)
22.0000	0.0000	0.00000	2631.99	0.00000	0.00000
1.0000	34.7178	2.96835	5231.58	2.96833	-0.00002
4.5000	34.6978	3.27464	5429.24	3.27466	0.00002
14.9999	34.6545	4.25385	6016.97	4.25386	0.00001
18.5000	34.6448	4.59807	6210.08	4.59806	-0.00001
24.0000	34.6345	5.15456	6509.85	5.15455	-0.00002
29.0000	34.6289	5.67507	6777.88	5.67508	0.00001
32.5000	34.6261	6.04656	6962.65	6.04663	0.00007

$$f = \text{Instrument Output(Hz)} * \sqrt{1.0 + \text{WBOTC} * t} / 1000.0$$

$$t = \text{temperature (°C)}; \quad p = \text{pressure (decibars)}; \quad \delta = \text{CTcor}; \quad \varepsilon = \text{CPcor};$$

$$\text{Conductivity (S/m)} = (g + h * f^2 + i * f^3 + j * f^4) / 10 (1 + \delta * t + \varepsilon * p)$$
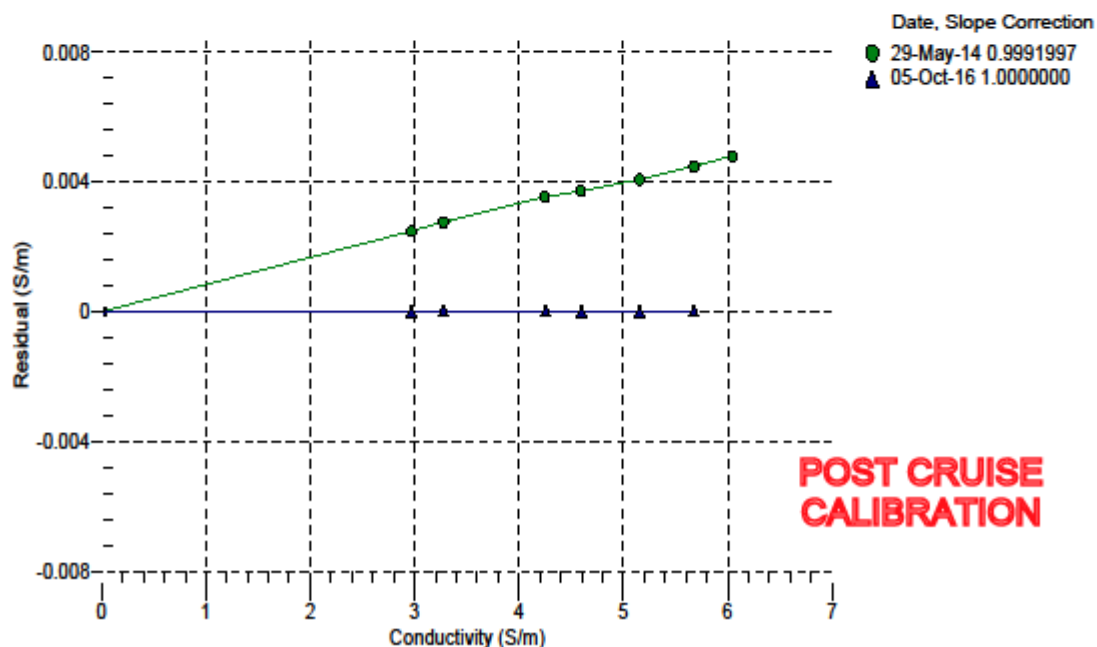
$$\text{Residual (Siemens/meter)} = \text{instrument conductivity} - \text{bath conductivity}$$




## Micro-TSG1

**SBE** SEA-BIRD ELECTRONICS, INC.  
13431 NE 20th St. Bellevue, Washington 98005 USA  
 Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

Temperature Calibration Report

Customer:	Lockheed Martin Antarctic Support		
Job Number:	86705	Date of Report:	2/22/2016
Model Number:	SBE 45	Serial Number:	4546167-0199

Temperature sensors are normally calibrated 'as received', without adjustments, allowing a determination sensor drift. If the calibration identifies a problem, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.

An 'as received' calibration certificate is provided, listing coefficients to convert sensor frequency to temperature. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients. The coefficient 'offset' allows a small correction for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair apply only to subsequent data.

'AS RECEIVED CALIBRATION' ☒ Performed ☐ Not Performed  
Date: 1/29/2016 Drift since last cal: -0.00074 Degrees Celsius/year  
Comments:

'FINAL CALIBRATION' ☒ Performed ☐ Not Performed  
Date: 2/19/2016 Drift since 02 Nov 13 -0.00079 Degrees Celsius/year  
Comments:

## Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0199  
CALIBRATION DATE: 19-Feb-16SBE 45 CONDUCTIVITY CALIBRATION DATA  
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter


## COEFFICIENTS:

g = -9.839079e-001  
h = 1.397390e-001  
i = -3.278767e-005  
j = 2.412783e-005CPcor = -9.5700e-008  
CTcor = 3.2500e-006  
WBOTC = -1.0552e-005

BATH TEMP (°C)	BATH SAL (PSU)	BATH COND (S/m)	INSTRUMENT OUTPUT (Hz)	INSTRUMENT COND (S/m)	RESIDUAL (S/m)
22.0000	0.0000	0.00000	2653.02	0.00000	0.00000
1.0000	34.6481	2.96295	5305.01	2.96295	-0.00000
4.5000	34.6281	3.26871	5505.90	3.26871	0.00000
15.0000	34.5846	4.24619	6103.19	4.24620	0.00001
18.5000	34.5748	4.58978	6299.43	4.58976	-0.00002
24.0000	34.5639	5.14521	6604.13	5.14522	0.00001
29.0000	34.5571	5.66462	6876.55	5.66462	-0.00000
32.5000	34.5537	6.03536	7064.36	6.03527	-0.00009

 $f = \text{Instrument Output(Hz)} * \sqrt{1.0 + \text{WBOTC} * t} / 1000.0$ t = temperature (°C); p = pressure (decibars);  $\delta = \text{CTcor}$ ;  $\epsilon = \text{CPcor}$ ;Conductivity (S/m) =  $(g + h * f^2 + i * f^3 + j * f^4) / 10 (1 + \delta * t + \epsilon * p)$ 

Residual (Siemens/meter) = instrument conductivity - bath conductivity

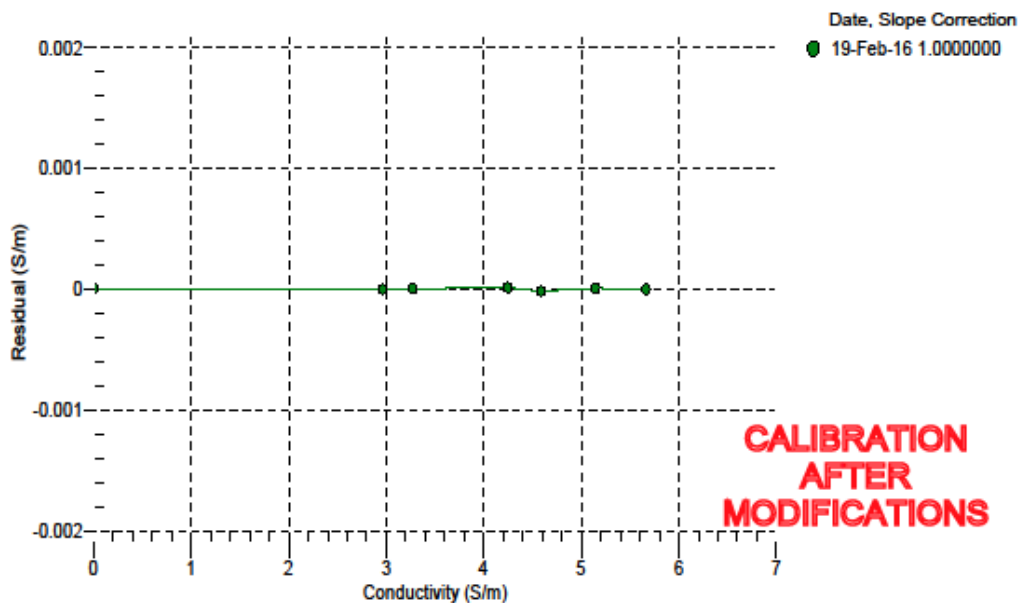

## Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0199  
CALIBRATION DATE: 19-Feb-16SBE 45 TEMPERATURE CALIBRATION DATA  
ITS-90 TEMPERATURE SCALE


## COEFFICIENTS:

$a_0 = 3.346026 \times 10^{-5}$   
 $a_1 = 2.683251 \times 10^{-4}$   
 $a_2 = -1.851289 \times 10^{-6}$   
 $a_3 = 1.425108 \times 10^{-7}$

BATH TEMP (° C)	INSTRUMENT OUTPUT (counts)	INST TEMP (° C)	RESIDUAL (° C)
1.0000	678437.9	1.0000	0.0000
4.5000	580549.3	4.4999	-0.0001
15.0000	370832.4	15.0000	-0.0000
18.5000	321323.4	18.5001	0.0001
24.0000	258039.6	24.0000	-0.0000
29.0000	212658.3	28.9999	-0.0001
32.5000	186333.4	32.5001	0.0001

 $n$  = Instrument Output (counts)Temperature ITS-90 (°C) =  $1 / \{a_0 + a_1[\ln(n)] + a_2[\ln^2(n)] + a_3[\ln^3(n)]\} - 273.15$ 

Residual (°C) = instrument temperature - bath temperature

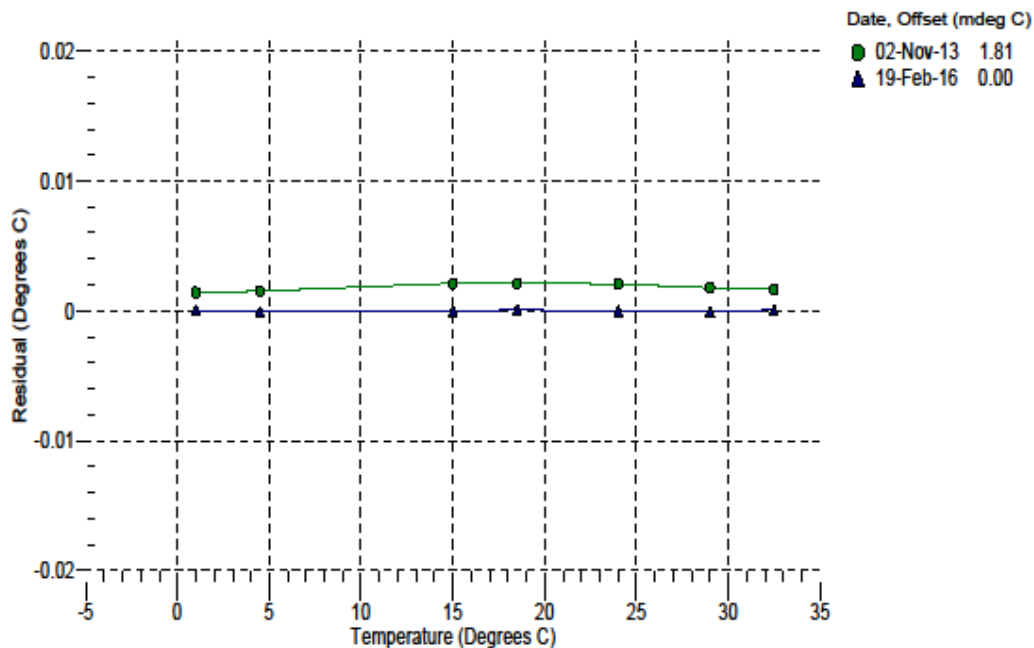

## Digital Remote Temp

**SEA-BIRD ELECTRONICS, INC.**

13431 NE 20th St. Bellevue, Washington 98005 USA

Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

**Temperature Calibration Report**

Customer:	Lockheed Martin Antarctic Support		
Job Number:	84324	Date of Report:	6/8/2015
Model Number	SBE 38	Serial Number:	3850449-0389

Temperature sensors are normally calibrated 'as received', without adjustments, allowing a determination sensor drift. If the calibration identifies a problem, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.

An 'as received' calibration certificate is provided, listing coefficients to convert sensor frequency to temperature. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients. The coefficient 'offset' allows a small correction for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair apply only to subsequent data.

**'AS RECEIVED CALIBRATION'**☒ Performed ☐ Not Performed

Date: 6/8/2015

Drift since last cal: +0.00071 Degrees Celsius/year

**Comments:**

The connector was upgraded.

**'CALIBRATION AFTER REPAIR'**☐ Performed ☒ Not Performed

Date:

Drift since Last cal: Degrees Celsius/year

**Comments:**

## Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0389  
CALIBRATION DATE: 08-Jun-15SBE 38 TEMPERATURE CALIBRATION DATA  
ITS-90 TEMPERATURE SCALE

## COEFFICIENTS:


$a_0 = 5.529089e-005$   
 $a_1 = 2.722899e-004$   
 $a_2 = -2.318547e-006$   
 $a_3 = 1.481909e-007$

BATH TEMP (ITS-90)	INSTRUMENT OUTPUT	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.5000	749636.8	-1.5000	0.0000
0.9999	667830.2	0.9999	-0.0000
4.5000	569749.8	4.4999	-0.0001
8.0000	487704.3	8.0000	0.0000
11.4999	418836.7	11.5000	0.0001
15.0000	360832.6	14.9999	-0.0001
18.4999	311816.7	18.4999	0.0000
21.9999	270263.8	22.0000	0.0001
25.5000	234929.8	25.4999	-0.0001
29.0000	204791.1	28.9999	-0.0001
32.4999	179008.3	32.5000	0.0001

$$\text{Temperature ITS-90} = 1/\{a_0 + a_1[\ln(n)] + a_2[\ln^2(n)] + a_3[\ln^3(n)]\} - 273.15 \text{ (}^\circ\text{C)}$$

Residual = instrument temperature - bath temperature

n = instrument output

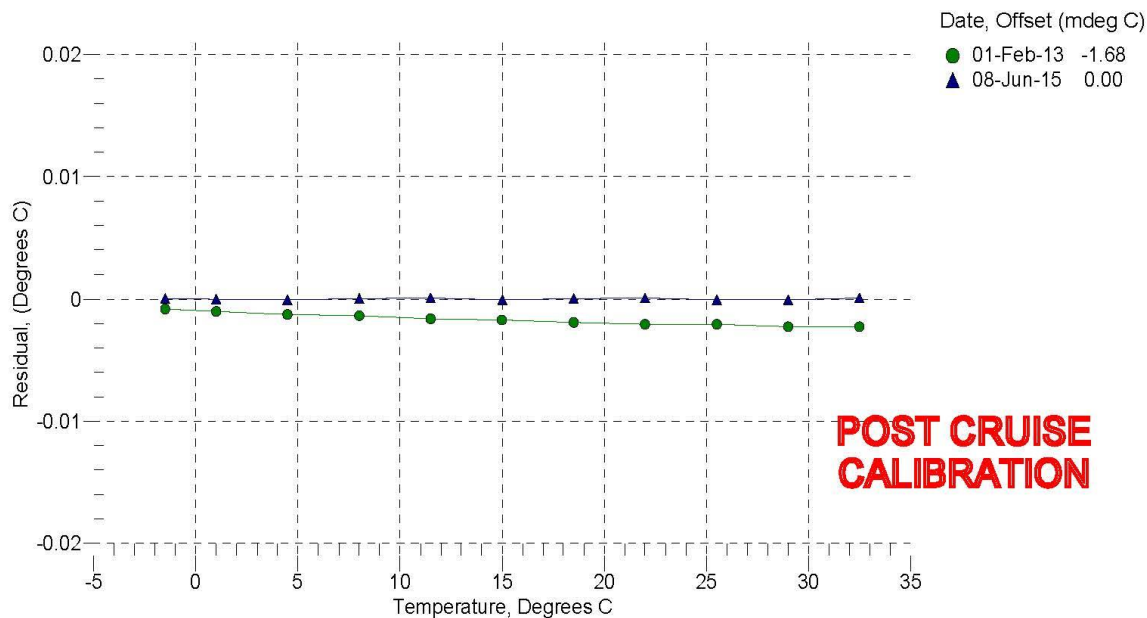

## Transmissometer

PO Box 518  
620 Applegate St.  
Philomath, OR 97370



(541) 829-5650  
Fax (541) 829-5277  
[www.wetlabs.com](http://www.wetlabs.com)

## C-Star Calibration

Date	7.8.15	S/N#	CST-889DR	Pathlength	25cm
<b>Analog output</b>					
$V_d$	0.058 V				
$V_{air}$	4.729 V				
$V_{ref}$	4.622 V				
Temperature of calibration water					24.1 °C
Ambient temperature during calibration					22.5 °C

Relationship of transmittance ( $Tr$ ) to beam attenuation coefficient ( $c$ ), and pathlength ( $x$ , in meters):  $Tr = e^{-cx}$

To determine beam transmittance:  $Tr = (V_{sig} - V_{dark}) / (V_{ref} - V_{dark})$

To determine beam attenuation coefficient:  $c = -1/x * \ln(Tr)$

$V_d$  Meter output with the beam blocked. This is the offset.

$V_{air}$  Meter output in air with a clear beam path.

$V_{ref}$  Meter output with clean water in the path.

Temperature of calibration water: temperature of clean water used to obtain  $V_{ref}$ .

Ambient temperature: meter temperature in air during the calibration.

$V_{sig}$  Measured signal output of meter.

Revision M

7/26/11

## Fluorometer

PO Box 518  
620 Applegate St.  
Philomath, OR 97370



(541) 929-5650  
Fax (541) 929-5277  
[www.wetlabs.com](http://www.wetlabs.com)

## ECO Chlorophyll Fluorometer Characterization Sheet

Date: 10/23/2015

S/N: FLRTD-4158

Chlorophyll concentration expressed in  $\mu\text{g/l}$  can be derived using the equation:

$$\text{CHL } (\mu\text{g/l}) = \text{Scale Factor} * (\text{Output} - \text{Dark Counts})$$

	Analog Range 1	Analog Range 2	Analog Range 4 (default)	Digital
Dark Counts	0.060	0.035	0.022 V	42 counts
Scale Factor (SF)	6	12	25 $\mu\text{g/l/V}$	0.0076 $\mu\text{g/l/count}$
Maximum Output	5.01	5.01	5.01 V	16380 counts
Resolution	0.8	0.8	0.8 mV	1.0 counts

Ambient temperature during characterization

21.3 °C

**Analog Range:** 1 (most sensitive, 0–4,000 counts), 2 (midrange, 0–8,000 counts), 4 (entire range, 0–16,000 counts).

**Dark Counts:** Signal output of the meter in clean water with black tape over detector.

**SF:** Determined using the following equation:  $\text{SF} = x \div (\text{output} - \text{dark counts})$ , where  $x$  is the concentration of the solution used during instrument characterization. SF is used to derive instrument output concentration from the raw signal output of the fluorometer.

**Maximum Output:** Maximum signal output the fluorometer is capable of.

**Resolution:** Standard deviation of 1 minute of collected data.

The relationship between fluorescence and chlorophyll-*a* concentrations *in-situ* is highly variable. The scale factor listed on this document was determined using a mono-culture of phytoplankton (*Thalassiosira weissflogii*). The population was assumed to be reasonably healthy and the concentration was determined by using the absorption method. To accurately determine chlorophyll concentration using a fluorometer, you must perform secondary measurements on the populations of interest. This is typically done using extraction-based measurement techniques on discrete samples. For additional information on determining chlorophyll concentration see "Standard Methods for the Examination of Water and Wastewater" part 10200 H, published jointly by the American Public Health Association, American Water Works Association, and the Water Environment Federation.

FLRTD-4158.xls

Revision J

3/17/08



## CTD

## Altimeter

Instrument Serial Number	51519
Sensor Type	500kHz Neptune
Altimeter Range (m)	100m
Certificate Number	49382

## Stage 1

Test the assembled altimeter in a body of water to ensure a signal is recieved at the minimum range. Taking direct readings from the unit immerse the head till it is roughly 0.1m from the bottom, readings should come through - if not then the signal is being saturated and there is a problem

To inhibit spurious readings set using:

#226;40

	Pass/Fail
Bench Test Min Range <0.1m	Pass

## Stage 2

Using a mini SVS or similar, measure the average sound velocity for the water in the tow tank and input the value in the cell below.

Enter the SOS	1484.385
---------------	----------

Input SOS value to the altimeter using:

#830;1484.3850

## Stage 3

Fit the altimeter into the calibration fixture and lower the assembly into the tank till it is about 0.5m down facing the far end of the tow tank and clamp in place. Using the distance markers on the wall align the front edge of the trolley with the datum line to set the front of the altimeter at stated distance from the wall.

To determine the Range Offset		
Distance m	Measured Range m	Measured Offset m
1	1.021	-0.021

## Stage 4: Enter the Offset Correction

#828;-0.0210

Stage 5 - Range Check after Offset Correction			
Distance m	Measured Range m	Measured Offset m	Pass/Fail
1	0.997	0.003	Pass
5	5	0	Pass

## Stage 6: Reset the SOS

#830;1500

Stage 7: Reset maximum range to 105m	Stage 8: Reset spurious range
#823;105 (500kHz units)	#226;0

Calibrated by:	J. Harper	Date:	07/10/2015
----------------	-----------	-------	------------



## Conductivity (primary)

## Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 2819  
CALIBRATION DATE: 20-Sep-16SBE 4 CONDUCTIVITY CALIBRATION DATA  
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

## COEFFICIENTS:


g = -1.02951064e+001  
h = 1.42205428e+000  
i = 9.24658304e-003  
j = -7.85335949e-004CPcor = -9.5700e-008 (nominal)  
CTcor = 3.2500e-006 (nominal)

BATH TEMP (°C)	BATH SAL (PSU)	BATH COND (S/m)	INSTRUMENT OUTPUT (kHz)	INSTRUMENT COND (S/m)	RESIDUAL (S/m)
0.0000	0.0000	0.00000	2.67278	0.00002	0.00002
-1.0000	34.6548	2.79278	5.13619	2.79257	-0.00021
1.0000	34.6551	2.96350	5.24953	2.96344	-0.00005
15.0000	34.6566	4.25409	6.03848	4.25474	0.00065
18.5000	34.6563	4.59943	6.23257	4.59953	0.00010
29.0001	34.6543	5.67877	6.80454	5.67727	-0.00151
32.5001	34.6476	6.04990	6.99227	6.05091	0.00101

f = Instrument Output (kHz)

t = temperature (°C); p = pressure (decibars);  $\delta$  = CTcor;  $\epsilon$  = CPcor;Conductivity (S/m) =  $(g + h * f^2 + i * f^3 + j * f^4) / (1 + \delta * t + \epsilon * p)$ 

Residual (Siemens/meter) = instrument conductivity - bath conductivity

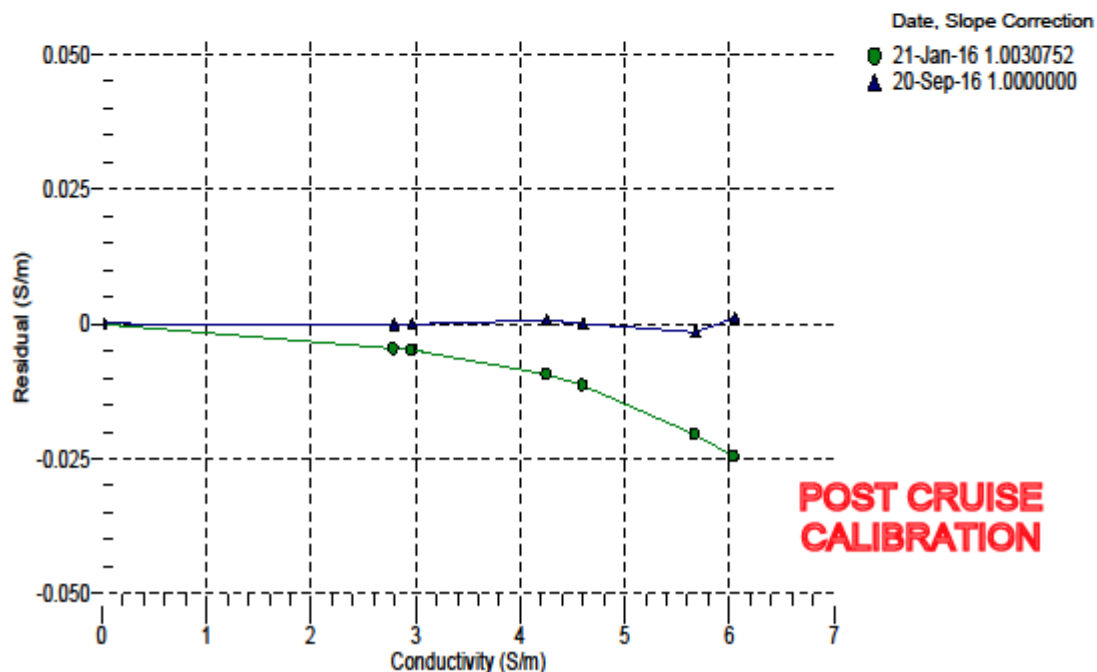

## Conductivity (secondary)

## Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 2569  
CALIBRATION DATE: 20-Sep-16SBE 4 CONDUCTIVITY CALIBRATION DATA  
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

## COEFFICIENTS:


g = -1.04785719e+001  
h = 1.58738716e+000  
i = 9.17747073e-005  
j = 9.25102032e-005CPcor = -9.5700e-008 (nominal)  
CTcor = 3.2500e-006 (nominal)

BATH TEMP (°C)	BATH SAL (PSU)	BATH COND (S/m)	INSTRUMENT OUTPUT (kHz)	INSTRUMENT COND (S/m)	RESIDUAL (S/m)
0.0000	0.0000	0.00000	2.56859	0.00000	0.00000
-1.0000	34.6548	2.79278	4.91464	2.79277	-0.00001
1.0000	34.6551	2.96350	5.02254	2.96351	0.00001
15.0000	34.6566	4.25409	5.77286	4.25408	-0.00001
18.5000	34.6563	4.59943	5.95753	4.59944	0.00001
29.0001	34.6543	5.67877	6.50068	5.67876	-0.00001
32.5001	34.6476	6.04990	6.67716	6.04991	0.00001

f = Instrument Output (kHz)

t = temperature (°C); p = pressure (decibars);  $\delta$  = CTcor;  $\epsilon$  = CPcor;Conductivity (S/m) =  $(g + h * f^2 + i * f^3 + j * f^4) / 10 (1 + \delta * t + \epsilon * p)$ 

Residual (Siemens/meter) = instrument conductivity - bath conductivity

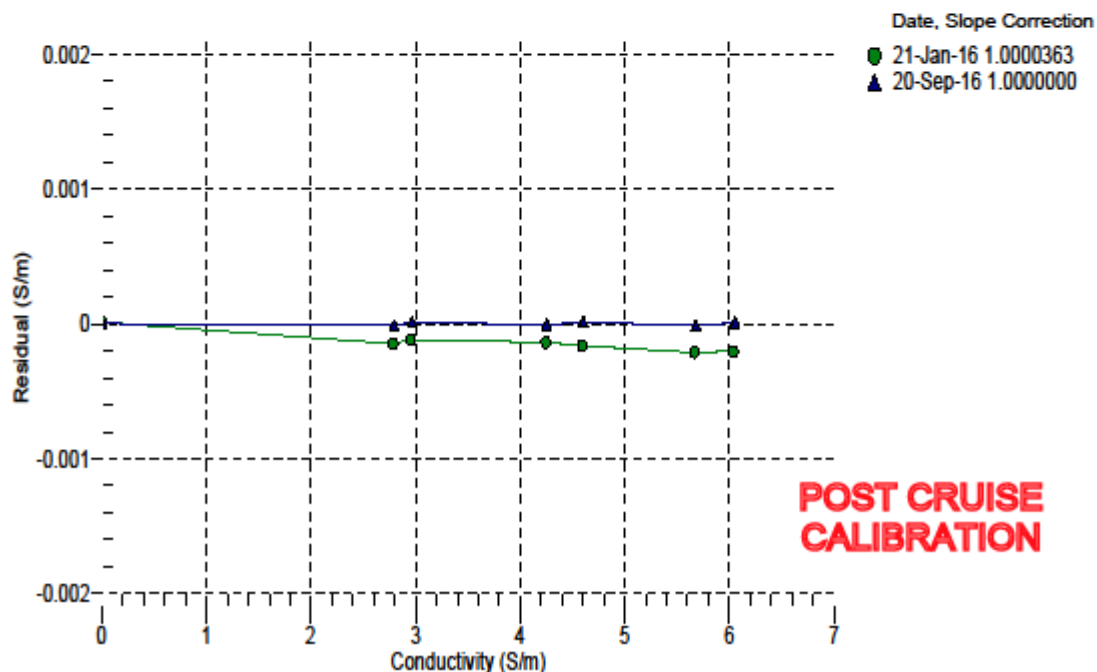

## Fluorometer

PO Box 518  
620 Applegate St.  
Philomath, OR 97370



(541) 929-5850  
Fax (541) 929-5277  
[www.wetlabs.com](http://www.wetlabs.com)

## ECO Chlorophyll Fluorometer Characterization Sheet

Date: 2/23/2015

S/N: FLRTD-397

Chlorophyll concentration expressed in µg/l can be derived using the equation:

$$\text{CHL } (\mu\text{g/l}) = \text{Scale Factor} * (\text{Output} - \text{Dark Counts})$$

	Analog Range 1	Analog Range 2	Analog Range 4 (default)	Digital
Dark Counts	0.107	0.065	0.044 V	67 counts
Scale Factor (SF)	6	13	26 µg/VV	0.0078 µg/l/count
Maximum Output	4.97	4.97	4.97 V	16330 counts
Resolution	0.7	0.7	0.7 mV	1.0 counts

Ambient temperature during characterization

22.3 °C

**Analog Range:** 1 (most sensitive, 0–4,000 counts), 2 (midrange, 0–8,000 counts), 4 (entire range, 0–16,000 counts).

**Dark Counts:** Signal output of the meter in clean water with black tape over detector.

**SF:** Determined using the following equation:  $SF = x \div (\text{output} - \text{dark counts})$ , where x is the concentration of the solution used during instrument characterization. SF is used to derive instrument output concentration from the raw signal output of the fluorometer.

**Maximum Output:** Maximum signal output the fluorometer is capable of.

**Resolution:** Standard deviation of 1 minute of collected data.

The relationship between fluorescence and chlorophyll-a concentrations *in-situ* is highly variable. The scale factor listed on this document was determined using a mono-culture of phytoplankton (*Thalassiosira weissflogii*). The population was assumed to be reasonably healthy and the concentration was determined by using the absorption method. To accurately determine chlorophyll concentration using a fluorometer, you must perform secondary measurements on the populations of interest. This is typically done using extraction-based measurement techniques on discrete samples. For additional information on determining chlorophyll concentration see "Standard Methods for the Examination of Water and Wastewater" part 10200 H, published jointly by the American Public Health Association, American Water Works Association, and the Water Environment Federation.

FLRTD-397

Revision J

3/17/08

## PAR

## CALIBRATION CERTIFICATE

### UNDERWATER PAR SENSOR WITH LOG AMPLIFIER

Calibration Date: 02/16/15		Job No.: R12136							
Model Number: QSP200L4S									
Serial Number: 4361									
Operator: TPC									
Standard Lamp: V-033(3/7/12)									
Operating Voltage Range: 6 to 15 VDC (+)									
Note: The QSP200L4S uses a log amplifier to measure the detector signal current with $V = \log I \text{ (Amps)} / I_{Ref}$ To calculate irradiance, use this formula									
<b>Irradiance = Calibration factor * (10<sup>A</sup>Light Signal Voltage - 10<sup>A</sup>Dark Voltage)</b>									
With the appropriate (solar corrected) Irradiance Calibration Factor:									
Dry Calibration Factor: 1.16E+13 quanta/cm <sup>2</sup> ·sec/"amps"		1.93E-05	μEinsteins/cm <sup>2</sup> ·sec/"amps"						
Wet Calibration Factor: 2.05E+13 quanta/cm <sup>2</sup> ·sec/"amps"		3.40E-05	μEinsteins/cm <sup>2</sup> ·sec/"amps"						
<b>Sensor Test Data and Results<sup>1)</sup></b>									
Sensor Supply Current (Dark): 75.5		mA							
Supply Voltage: 6		Volts							
Lamp Integrated PAR Irradiance: 9.34E+15 quanta/cm <sup>2</sup> ·sec		0.01551	μEinsteins/cm <sup>2</sup> ·sec						
SC3 Immersion Coefficient: 0.5864		Scalar Correction: 1	PAR Solar Correction: 1.0000						
Nominal Filter-OD	Calibrated Trans.	Sensor Voltage	Measured Trans.	Measured Signal (Amps)	Estimated Signal (Amps)	Calc. Output (Volts)	Error (Volts)	Error (%)	Test Irrad (quanta/cm <sup>2</sup> ·sec)
No Filter	100.00%	2.907	100.00%	8.07E-08	8.07E-08	2.908	0.001	0.0	9.34E+15
0.3	38.13%	2.486	38.09%	2.91E-08	2.91E-08	2.467	0.001	0.0	3.37E+15
0.5	27.63%	2.351	27.65%	2.23E-08	2.23E-08	2.351	0.000	-0.2	2.58E+15
1	9.27%	1.881	9.26%	7.48E-09	7.48E-09	1.883	0.002	0.2	8.84E+14
2	1.11%	1.013	1.06%	8.79E-10	8.96E-10	1.021	0.008	2.0	1.02E+14
3	0.05%	0.322	0.07%	5.78E-11	4.31E-11	0.291	-0.031	-25.2	6.67E+12
Dark Before: 0.183 Volts									
Light - No Filter Hdr: 2.908 Volts				$I_{Ref} = 1.00E-10$ Amps					
Dark After - NFH: 0.183 Volts				$I_{Dark} = 1.52E-10$ Amps		RG780		0.22	
Average Dark: 0.183 Volts				$10^{V_{Dark}} = 1.524053$ Amps					

Notes:

1. Annual calibration is recommended.
2. The collector should be cleaned frequently with alcohol.
- 4) This section is for internal use and for more advanced analysis.

## Pressure Sensor

**Sea-Bird Electronics, Inc.**13431 NE 20<sup>th</sup> St. Bellevue, Washington 98005 USA  
www.seabird.com

Phone: (425) 643-9866

Fax: (425) 643-9954

Email: seabird@seabird.com

**Pressure Test Certificate**

Test Date: 05/02/16

Description: SBE-9plus CTD

**Sensor Information:**

Model Number: 09

Serial Number: 1281

**Pressure Test Protocol:**


Low Pressure Test: 40 PSI Held For: 15 Minutes

High Pressure Test: 10000 PSI Held For: 15 Minutes

Passed Test: Yes

Tested By: nd

High pressure is  
generally equal  
to the maximum  
depth rating of  
the instrument

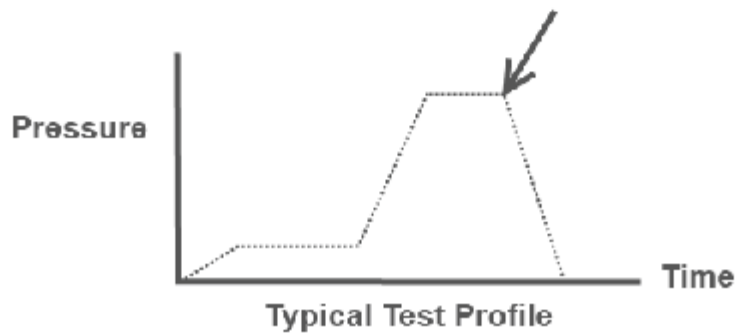



**SEA-BIRD ELECTRONICS, INC.**  
 13431 NE 20<sup>th</sup> St, Bellevue Washington 98005 USA  
 Phone: (425) 643-9866 Fax: (425) 643-9954 Email: seabird@seabird.com

**Digiquartz Pressure Calibration dP/dT Corrected Coefficients**  
*(Changed coefficients are posted in italics)*

Pressure Transducer Serial Number: 136428  
 Original Calibration Date: 02-May-16  
 Date of Correction: 2016-05-17  
 Installed in: SBE 9Plus S/N 1281

**PRESSURE COEFFICIENTS**

<i>C1</i>	<i>-41607.74</i>	<i>psia</i>
<i>C2</i>	<i>-0.4184703</i>	<i>psia/deg C</i>
<i>C3</i>	<i>1.315700e-002</i>	<i>psia/deg C<sup>2</sup></i>
 D1	 3.510400e-002	
D2	0.000000e+000	
 <i>T1</i>	 <i>30.13996</i>	 <i>μsec</i>
<i>T2</i>	<i>-3.93972e-04</i>	<i>μsec/deg C</i>
<i>T3</i>	<i>4.255700e-006</i>	<i>μsec/deg C<sup>2</sup></i>
<i>T4</i>	<i>2.107770e-009</i>	<i>μsec/deg C<sup>3</sup></i>
<i>T5</i>	<i>0.000000e+000</i>	

Slope = 1.0  
 Offset = 0.0

Corrected at Sea-Bird Electronics as per Paroscientific Calibration and Sea-Bird Electronics dP/dT tests. The original calibration from Paroscientific assumes an operating temperature range of 0 to 125 degrees C. dP/dT correction adjusts this operating range to a nominal range of 0 to 22 degrees C. This increases the accuracy of the transducer in this temperature range.

NOTE: Original coefficients from Paroscientific are attached to this form for informational purposes and should not be used.

## Dissolved Oxygen (primary)

## Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0186  
CALIBRATION DATE: 14-Sep-16

## SBE 43 OXYGEN CALIBRATION DATA

## COEFFICIENTS:

Soc = 0.4481

Voffset = -0.5085

Tau20 = 1.16

A = -5.3178e-003

B = 3.0886e-004

C = -4.5954e-008

E nominal = 0.036

## NOMINAL DYNAMIC COEFFICIENTS

D1 = 1.92634e-4

D2 = -4.64803e-2

H1 = -3.300000e-2

H2 = 5.00000e+3

H3 = 1.45000e+3


BATH OXYGEN (ml/l)	BATH TEMPERATURE (°C)	BATH SALINITY (PSU)	INSTRUMENT OUTPUT (volts)	INSTRUMENT OXYGEN (ml/l)	RESIDUAL (ml/l)
1.13	6.00	0.00	0.803	1.12	-0.00
1.13	2.00	0.00	0.770	1.13	-0.00
1.15	12.00	0.00	0.858	1.15	-0.00
1.15	20.00	0.00	0.922	1.16	0.00
1.16	26.00	0.00	0.970	1.16	0.00
1.17	30.00	0.00	1.005	1.17	0.00
3.88	2.00	0.00	1.411	3.88	0.00
3.89	6.00	0.00	1.528	3.89	-0.00
3.91	12.00	0.00	1.696	3.90	-0.00
3.91	26.00	0.00	2.060	3.91	0.00
3.91	20.00	0.00	1.908	3.91	-0.00
3.92	30.00	0.00	2.175	3.93	0.00
6.63	30.00	0.00	3.323	6.63	-0.00
6.64	2.00	0.00	2.055	6.64	0.00
6.65	6.00	0.00	2.249	6.65	-0.00
6.65	26.00	0.00	3.150	6.65	-0.00
6.66	12.00	0.00	2.535	6.66	0.00
6.66	20.00	0.00	2.893	6.66	0.00

V = instrument output (volts); T = temperature (°C); S = salinity (PSU); K = temperature (°K)

Oxsol(T,S) = oxygen saturation (ml/l); P = pressure (dbar)

Oxygen (ml/l) = Soc \* (V + Voffset) \* (1.0 + A \* T + B \* T<sup>2</sup> + C \* T<sup>3</sup>) \* Oxsol(T,S) \* exp(E \* P / K)

Residual (ml/l) = instrument oxygen - bath oxygen

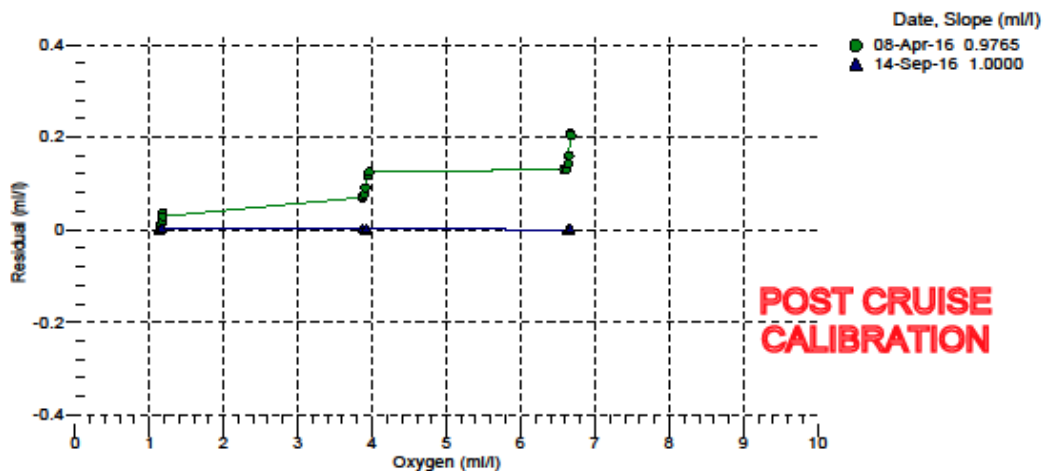



## Pump (primary)

<b>SBE</b>		<b>SEA-BIRD ELECTRONICS, INC.</b>	
13431 NE 20th St. Bellevue, Washington 98005 USA			
Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com			
<b>Service</b>		<b>RMA Number</b> 81844	
<b>Report</b>			
<b>Customer Information:</b>			
<b>Company</b>	Lockheed Martin Antarctic Support	<b>Date</b>	3/14/2015
<b>Contact</b>	Dave Morehouse		
<b>PO Number</b>	4900057588		
<b>Serial Number</b>	051626		
<b>Model Number</b>	SBE 05T		
<b>Services Requested:</b>			
1. Evaluate/Repair Instrumentation. 2. Install wet-pluggable connector.			
<b>Problems Found:</b>			
1. Unit was upgraded from impulses to subcon wet connector.			
<b>Services Performed:</b>			
1. Performed initial diagnostic evaluation. 2. Installed NEW two pin wet-pluggable bulkhead connector(s). 3. Performed internal inspection and O-ring and thrust washer replacements. 4. Performed hydrostatic pressure test.			
<b>Special Notes:</b>			

Saturday, March 14, 2015

Page 5 of 8



## Pump (secondary)

<b>SBE</b>		<b>SEA-BIRD ELECTRONICS, INC.</b>	
13431 NE 20th St. Bellevue, Washington 98005 USA			
Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com			
<b>Service</b>		<b>RMA Number</b> 81844	
<b>Report</b>			
<b>Customer Information:</b>			
<b>Company</b>	Lockheed Martin Antarctic Support	<b>Date</b>	3/14/2015
<b>Contact</b>	Dave Morehouse		
<b>PO Number</b>	4900057588		
<b>Serial Number</b>	051627		
<b>Model Number</b>	SBE 05T		
<b>Services Requested:</b>			
1. Evaluate/Repair Instrumentation. 2. Install wet-pluggable connector.			
<b>Problems Found:</b>			
1. Unit was upgraded from impules to subcon wet connector.			
<b>Services Performed:</b>			
1. Performed initial diagnostic evaluation. 2. Installed NEW two pin wet-pluggable bulkhead connector(s). 3. Performed internal inspection and O-ring and thrust washer replacements. 4. Performed hydrostatic pressure test.			
<b>Special Notes:</b>			

Saturday, March 14, 2015

Page 6 of 8

## Temperature (primary)

## Temperature Calibration Report

### STS/ODF Calibration Facility

SENSOR SERIAL NUMBER: 4209

CALIBRATION DATE: 12-Sep-2016

Mfg: SEABIRD Model: 03

Previous cal: 18-Nov-15

Calibration Tech: CAL


ITS-90_COEFFICIENTS	IPTS-68_COEFFICIENTS ITS-T90	
g = 4.34644284E-3	a = 4.34663760E-3	
h = 6.29342788E-4	b = 6.29548818E-4	
i = 2.01664652E-5	c = 2.01973913E-5	
j = 1.53546108E-6	d = 1.53681949E-6	
f0 = 1000.0	Slope = 1.0	Offset = 0.0

Calibration Standard: Mfg: Isotech Model: MicroK100 s/n: 291088-2

Temperature ITS-90 =  $1/[g+h[\ln(f_0/f)]+i[\ln^2(f_0/f)]+j[\ln^3(f_0/f)]] - 273.15$  (°C)Temperature IPTS-68 =  $1/[a+b[\ln(f_0/f)]+c[\ln^2(f_0/f)]+d[\ln^3(f_0/f)]] - 273.15$  (°C)

T68 = 1.00024 \* T90 (-2 to -35 Deg C)

SBE3 Freq	SPRT ITS-T90	SBE3 ITS-T90	SPRT-SBE3 OLD Coefs	SPRT-SBE3 NEW Coefs
2986.3781	-1.4130	-1.4132	0.00082	0.00015
3161.4909	1.0915	1.0917	0.00046	-0.00014
3419.0148	4.5980	4.5982	0.00038	-0.00016
3691.4808	8.1059	8.1059	0.00058	0.00004
3979.3740	11.6154	11.6152	0.00072	0.00016
4282.1891	15.1156	15.1156	0.00062	0.00003
4602.1685	18.6278	18.6278	0.00062	0.00000
4938.3467	22.1363	22.1363	0.00063	-0.00000
5291.6471	25.6467	25.6468	0.00055	-0.00009
5662.0140	29.1548	29.1549	0.00054	-0.00005
6050.3428	32.6656	32.6656	0.00056	0.00007

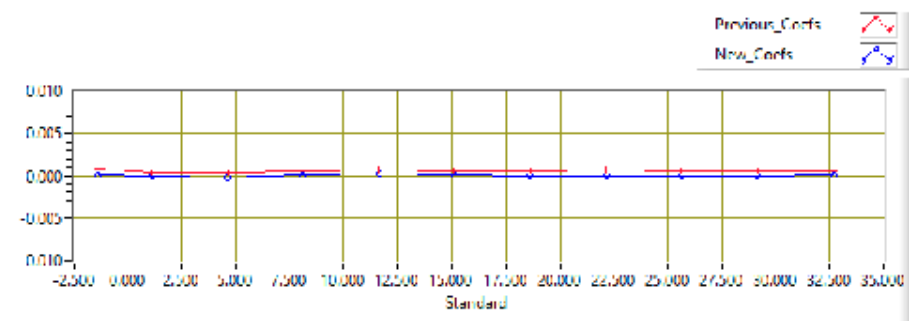

## Temperature (Secondary)

## Temperature Calibration Report

### STS/ODF Calibration Facility

**SENSOR SERIAL NUMBER:** 5844  
**CALIBRATION DATE:** 12-Sep-2016  
**Mfg:** SEABIRD **Model:** 03  
**Previous cal:** 18-Nov-15  
**Calibration Tech:** CAL

ITS-90_COEFFICIENTS	IPTS-68_COEFFICIENTS	
	ITS-T90	
<b>g</b> = 4.36553148E-3	<b>a</b> = 4.36573253E-3	
<b>h</b> = 6.29971788E-4	<b>b</b> = 6.30179520E-4	
<b>i</b> = 2.00553720E-5	<b>c</b> = 2.00863167E-5	
<b>j</b> = 1.50462745E-6	<b>d</b> = 1.50596866E-6	
<b>f0</b> = 1000.0	<b>Slope</b> = 1.0	<b>Offset</b> = 0.0


Calibration Standard: Mfg: Isotech Model: MicroK100 s/n: 291088-2

Temperature ITS-90 =  $1/[g+h[\ln(f_0/f)]+i[\ln^2(f_0/f)]+j[\ln^3(f_0/f)]] - 273.15$  (°C)

Temperature IPTS-68 =  $1/[a+b[\ln(f_0/f)]+c[\ln^2(f_0/f)]+d[\ln^3(f_0/f)]] - 273.15$  (°C)

T68 = 1.00024 \* T90 (-2 to -35 Deg C)

SBE3 Freq	SPRT ITS-T90	SBE3 ITS-T90	SPRT-SBE3 OLD Coefs	SPRT-SBE3 NEW Coefs
3080.3338	-1.4130	-1.4132	0.00093	0.00014
3261.0068	1.0915	1.0917	0.00060	-0.00014
3526.7023	4.5980	4.5981	0.00059	-0.00014
3807.8148	8.1059	8.1059	0.00077	0.00002
4104.8361	11.6154	11.6153	0.00093	0.00014
4417.2419	15.1156	15.1156	0.00091	0.00005
4747.3553	18.6278	18.6278	0.00092	0.00001
5094.1758	22.1363	22.1364	0.00092	-0.00004
5458.6432	25.6467	25.6467	0.00092	-0.00005
5840.7209	29.1548	29.1549	0.00089	-0.00006
6241.3151	32.6656	32.6656	0.00093	0.00007

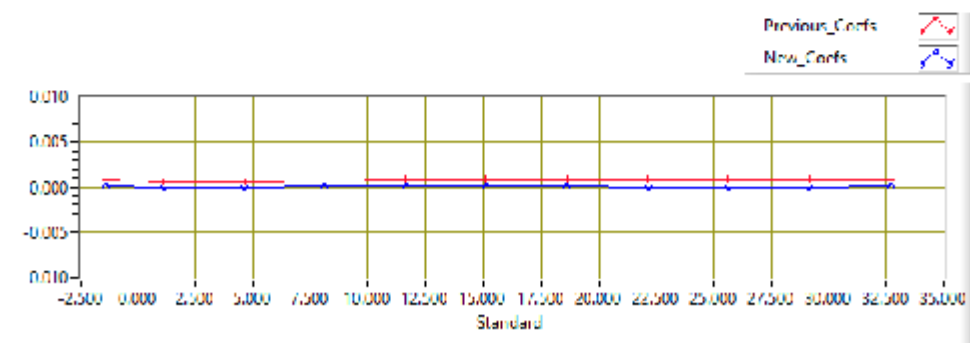

## Transmissometer

PO Box 518  
620 Applegate St.  
Philomath, OR 97370



(541) 829-5650  
Fax (541) 829-5277  
[www.wetlabs.com](http://www.wetlabs.com)

## C-Star Calibration

Date	7.27.15	S/N#	CST-557DR	Pathlength	25cm
		Analog output	Digital output		
$V_d$		0.007 V	0 counts		
$V_{air}$		4.766 V	15628 counts		
$V_{ref}$		4.700 V	15410 counts		
Temperature of calibration water				23.1	°C
Ambient temperature during calibration				22.9	°C

Relationship of transmittance ( $Tr$ ) to beam attenuation coefficient ( $c$ ), and pathlength ( $x$ , in meters):  $Tr = e^{-cx}$

To determine beam transmittance:  $Tr = (V_{sig} - V_{dark}) / (V_{ref} - V_{dark})$

To determine beam attenuation coefficient:  $c = -1/x * \ln(Tr)$

$V_d$  Meter output with the beam blocked. This is the offset.

$V_{air}$  Meter output in air with a clear beam path.

$V_{ref}$  Meter output with clean water in the path.

Temperature of calibration water: temperature of clean water used to obtain  $V_{ref}$ .

Ambient temperature: meter temperature in air during the calibration.

$V_{sig}$  Measured signal output of meter.

Revision L

6/9/09