

Layout No:
Circuit Diagram No:
Program Version: 5.2.1

Product: Conductivity Sensor 4319A
Serial No: 1297

1. Visual and Mechanical Checks:

- 1.1. Soldering quality
- 1.2. Visual surface
- 1.3. Galvanic isolation between housing and electronics

2. Current Drain and Voltages:

- | | |
|---|---------|
| 2.1. RS232 average current drain at 0.5Hz sampling (max: 25mA) | 18.0 mA |
| 2.2. RS232 peak current drain at 0.5Hz sampling | 75.0 mA |
| 2.3. RS232 current drain in sleep (max: 180µA) | 114 µA |
| 2.4. CANBus average current drain at 0.5Hz sampling (max: 25mA) | 18.0 mA |
| 2.5. CANBus peak current drain at 0.5Hz sampling | 75 mA |
| 2.6. CANBus current drain in sleep (max: 180µA) | 96.0 µA |
| 2.7. DSP voltage, (3.3 ±0.15V) | 3.30 V |
| 2.8. Excitation driver voltage, (3.3 ±0.15V) | 3.31 V |
| 2.9. Flash/RS232 driver voltage, (1.8 ±0.05V) | 1.80 V |

3. Electronic performance test:

- | | |
|---|-----------|
| 3.1. Average of Receiver readings (0 ±400mV) | 318 mV |
| 3.2. Standard Deviation of Receiver readings (max: 60mV) | 9 mV |
| 3.3. Cross-talk voltage with open loop (max: 550mV) | -252 mV |
| 3.4. Amplification (Zamp) with 0.2mS loop/5000 Ω (1200-2000) | 1692 mV |
| 3.5. Reading (CompValue) with open loop/0mS (1000 – 2000) | 1582 lsb |
| 3.6. Reading (CompValue) with 14.286mS loop/70Ω (50000 – 60000) | 52009 lsb |
| 3.7. CANBus Output test with 1 mS loop/1000 | |

4. Temperature cycling test:

- 4.1. Temperature cycling test in chamber (0-50°C)

5. Temperature test (2 – 35°C):

- | | |
|--|--------|
| 5.1. Raw data temperature drift with 14.286mS loop/70Ω loop
in High Range (max 500) | 12 lsb |
|--|--------|

6. Pressure test (0 – 60MPa):

- 6.1. Raw data drift with 14.286mS 70Ω loop in High Range (max 8)

Date: 20 May 2015

Sign:



Ingemar Nerhus, Production Engineer

Calibration Date: 04 Sep 2015
Product: Conductivity Sensor 4319A

Serial No: 1297

This is to certify that this product has been calibrated using the following instruments:

ASL Digital Thermometer model F250 Serial No.06792/06
Platinum Resistance Thermometer Serial No.2H1072/1
Calibration Bath model FNT 321-1-40 1
Aanderaa Active Loop 22

Parameter: Temperature

Calibration points and readings:

Temperature (°C)	1.157	12.117	24.126	36.094
Reading (mV)	2.42418E+03	2.11252E+03	1.74347E+03	1.38652E+03

Giving these coefficients


Index	0	1	2	3
TempCoef	1.11541E02	-8.31776E-02	2.77149E-05	-5.02719E-09

Parameter: Conductance linearization and temperature compensation

Giving these coefficients

Index	0	1	2	3
R1Coef0	8.98843E00	3.69068E-04	-7.02272E-07	-4.44359E-08
R1Coef1	8.98843E00	3.69068E-04	-7.02272E-07	-4.44359E-08
R1Coef2	-2.98686E-02	1.43465E-04	1.34772E-05	-3.21444E-07
R1Coef3	-5.70219E-02	-4.50741E-03	2.87448E-04	-4.42506E-06
R1Coef4	-4.18222E-02	-3.68675E-03	3.86681E-05	3.82879E-07
R1Coef5	2.80883E-01	2.12957E-02	-1.58851E-03	2.55826E-05
R1Coef6	1.90598E-01	1.06628E-02	-3.42565E-04	3.04339E-06
R1Coef7	-4.93779E-01	-4.17544E-02	3.21951E-03	-5.22957E-05
R1Coef8	-1.89786E-01	-8.33447E-03	3.89156E-04	-4.55700E-06
R1Coef9	3.36246E-01	2.76556E-02	-2.16368E-03	3.52160E-05

Error graph:

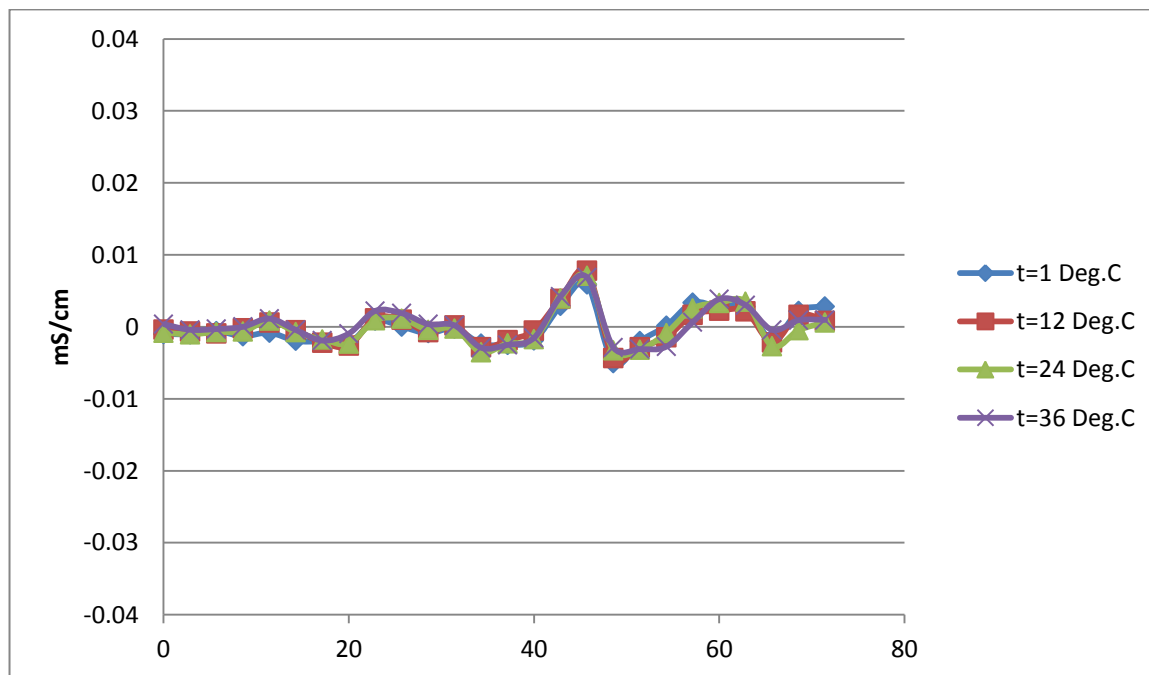

Product: Conductivity Sensor 4319A

Serial No: 1297

Parameter: Conductivity

Reference reading (mS/cm)	4.97850E+01
Conductance reading (mS)	1.08524E+01

Giving following cell coefficient

CellCoef	4.629
----------	-------

Date: 04 Sep 2015

Sign:

Tor-Ove Kvalvaag

Tor-Ove Kvalvaag, Calibration Engineer

Product: Conductivity Sensor 4319A

Certificate No: 1077871311297

Serial No: 1297

Date: 20.05.2015

This is to certify that this product has been pressure tested with the following instrument, and we confirm that no irregularities were found during the test:

Autoklav 800 bar – sn: 0210005

Pressure readings:

Pressure (Bar)	Pressure time (hour)
600	14

Date: 20 May 2015

Sign:



Ingemar Nerhus, Production Engineer